
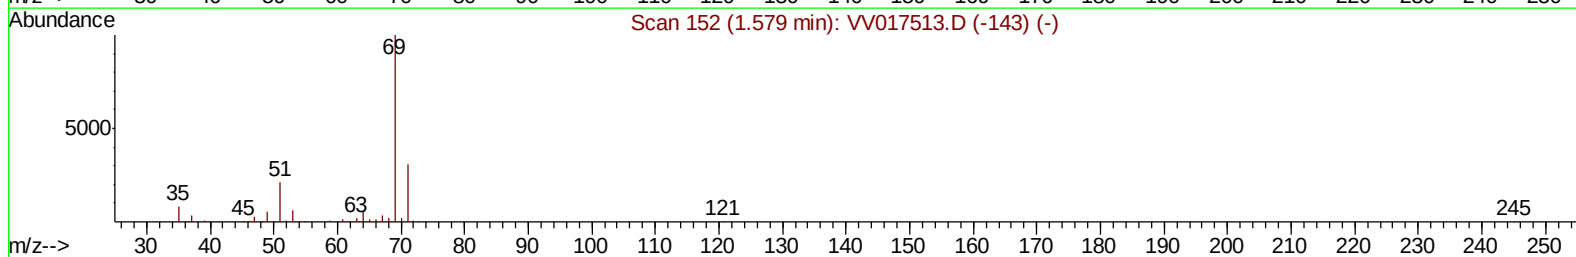
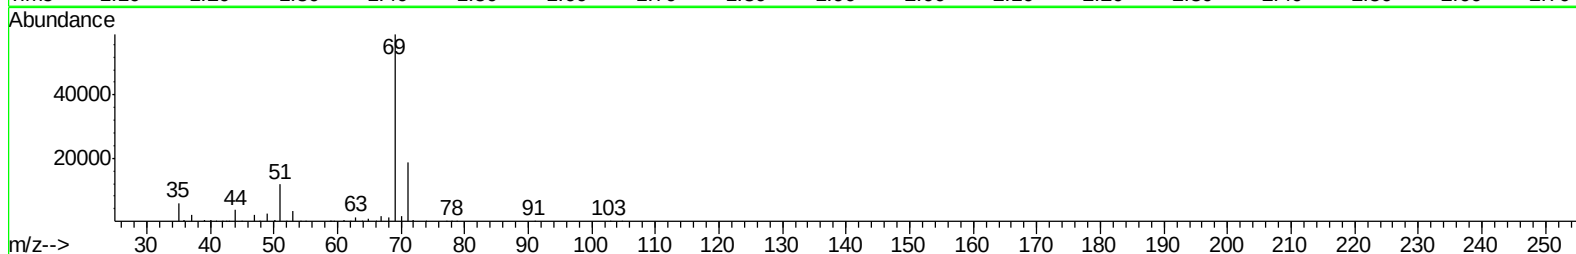


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
Data File : VV017533.D
Acq On : 17 Jul 2020 19:00
Operator : SY/MD
Sample : L3336-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Jul 18 05:11:36 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 18 05:06:25 2020
Response via : Initial Calibration

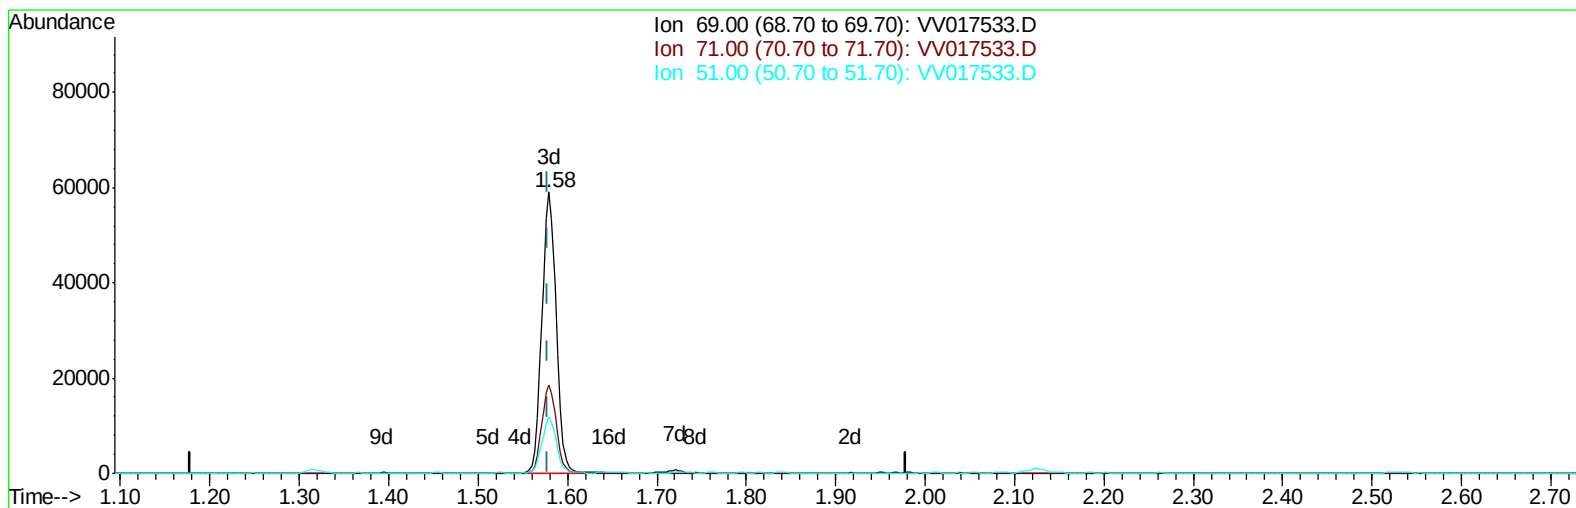

TIC: VV017533.D

(7) Chloroethane-d5 (S)

1.579min (+0.000) 53.86ug/L m

response 65441

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	0.07#
51.00	31.70	0.10#
0.00	0.00	0.00