

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
 Data File : VV0717518.D
 Acq On : 17 Jul 2020 12:25
 Operator : SY/MD
 Sample : L3336-19
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 FB(071520)

Quant Time: Jul 18 05:27:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 18 05:06:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	313096	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	294812	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	158292	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	78263	48.02	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	96.04%
7) Chloroethane-d5	1.58	69	69873	61.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	122.04%
11) 1,1-Dichloroethene-d2	2.12	63	140431	38.05	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.10%
21) 2-Butanone-d5	3.91	46	103535	93.00	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.00%
24) Chloroform-d	4.38	84	161529	42.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.68%
26) 1,2-Dichloroethane-d4	5.06	65	121906	47.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.22%
32) Benzene-d6	5.08	84	298733	46.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.82%
36) 1,2-Dichloropropane-d6	6.10	67	91252	49.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.52%
41) Toluene-d8	7.34	98	277916	45.39	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.78%
43) trans-1,3-Dichloropropene-	7.64	79	49691	46.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.10%
47) 2-Hexanone-d5	8.11	63	82194	109.21	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.21%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	133235	51.74	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.48%
64) 1,2-Dichlorobenzene-d4	11.65	152	129897	49.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.16%


Target Compounds					Ovalue
13) Acetone	2.20	43	12428	8.201 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071720\
Data File : VV017518.D
Acq On : 17 Jul 2020 12:25
Operator : SY/MD
Sample : L3336-19
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
FB(071520)

Quant Time: Jul 18 05:27:21 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 18 05:06:25 2020
Response via : Initial Calibration

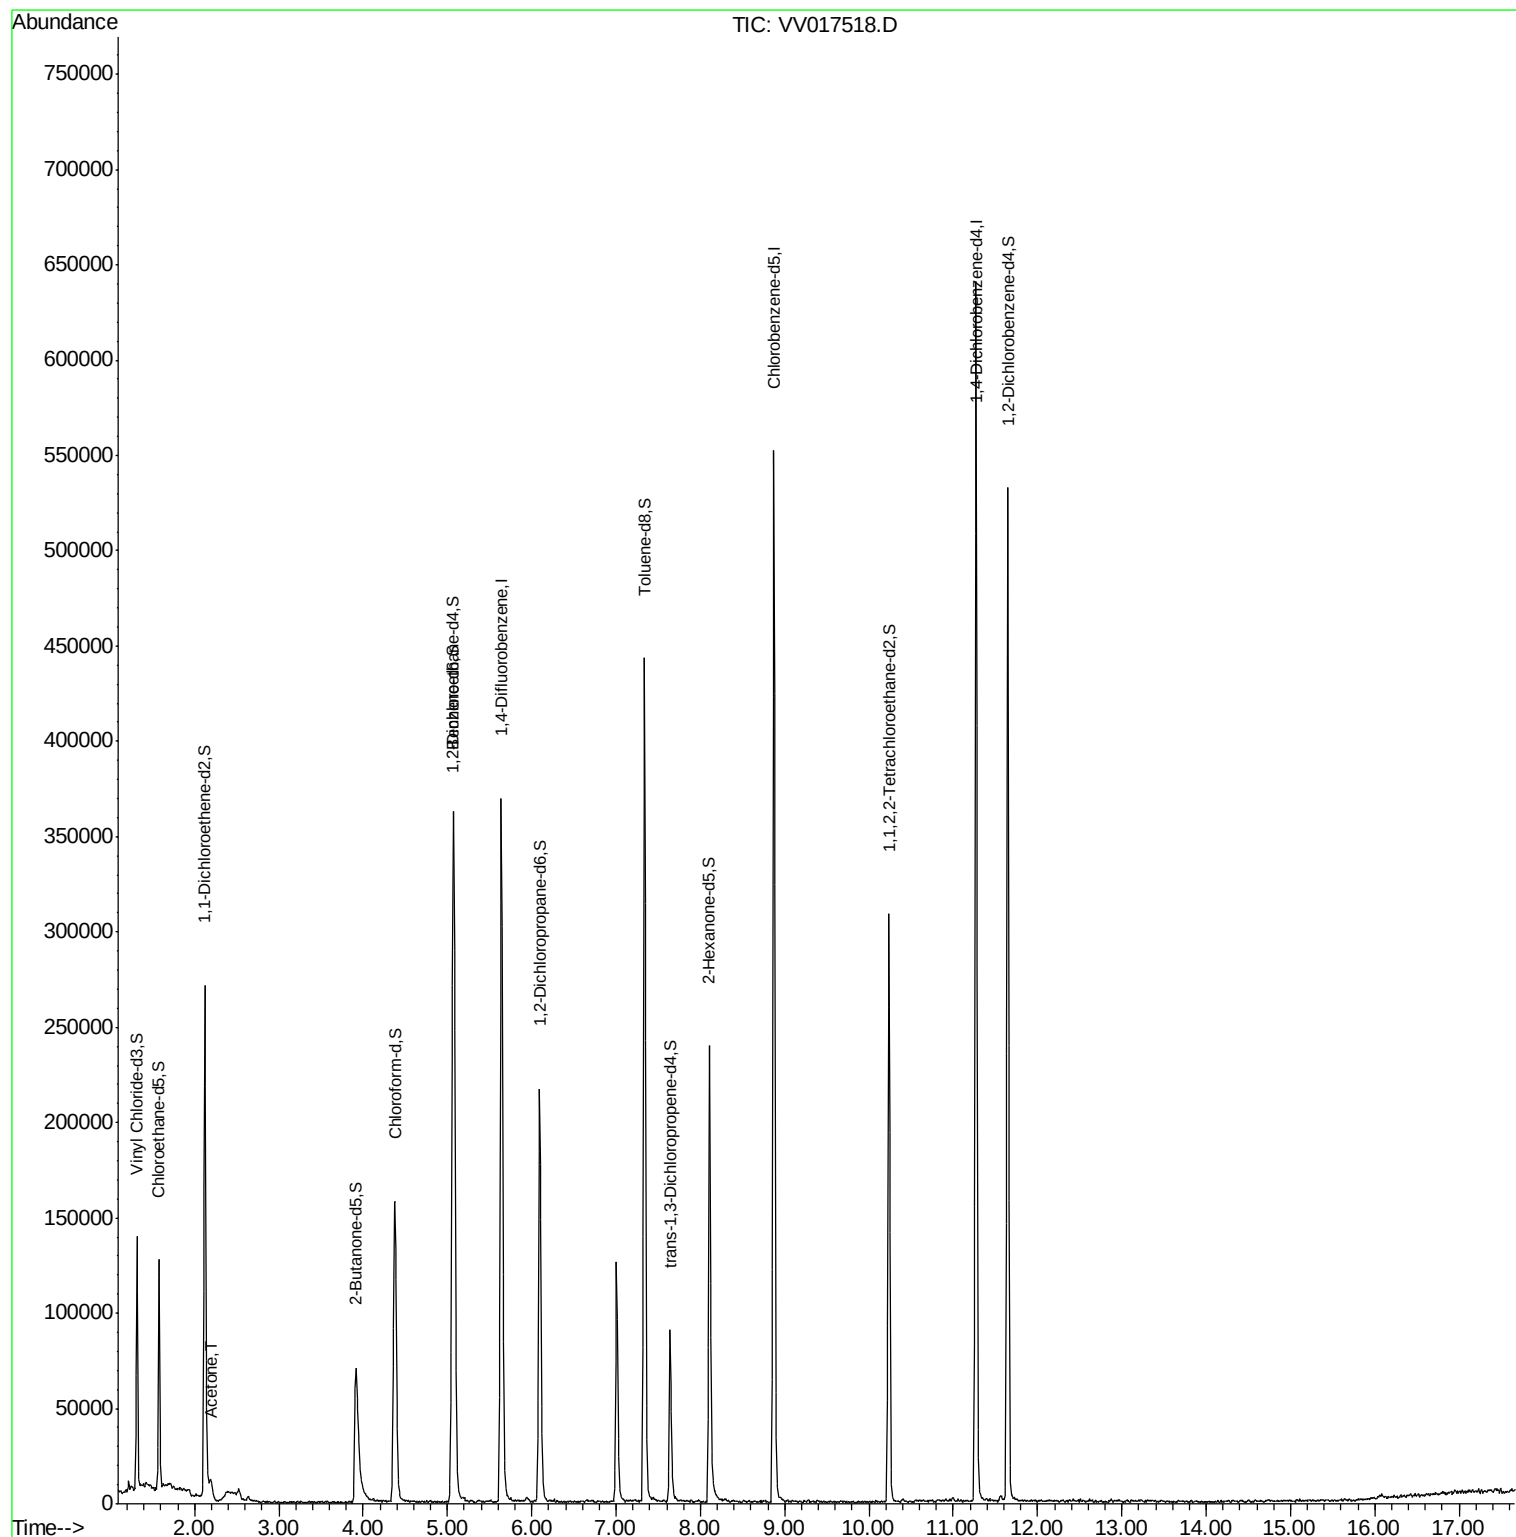

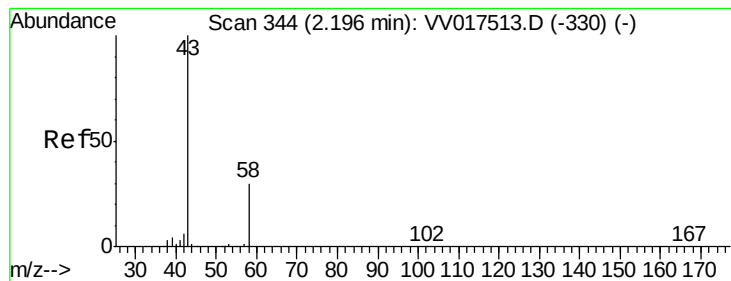

#13
 Acetone
 Concen: 8.201 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. 0.00 min
 Lab File: VV017518.D
 Acq: 17 Jul 2020 12:25

Instrument :
 MSVOA_V
 ClientSampleId :
 FB(071520)

Tot Ion: 43 Resp: 12428
 Ion Ratio Lower Upper
 43 100
 58 29.7 0.0 56.0

