

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
 Data File : VV017527.D
 Acq On : 17 Jul 2020 15:54
 Operator : SY/MD
 Sample : L3336-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-1

Quant Time: Jul 18 05:59:42 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jul 18 05:06:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	246717	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	243713	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	116186	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	78400	61.04	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	122.08%
7) Chloroethane-d5	1.58	69	73192	81.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	162.24%#
11) 1,1-Dichloroethene-d2	2.12	63	153380	52.74	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	105.48%
21) 2-Butanone-d5	3.91	46	103874	118.40	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	118.40%
24) Chloroform-d	4.38	84	173527	58.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	116.82%
26) 1,2-Dichloroethane-d4	5.06	65	128336	62.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	125.88%#
32) Benzene-d6	5.08	84	307817	58.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	116.94%
36) 1,2-Dichloropropane-d6	6.09	67	88944	58.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	117.34%
41) Toluene-d8	7.34	98	286549	56.61	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.22%
43) trans-1,3-Dichloropropene-	7.64	79	52160	59.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	118.22%
47) 2-Hexanone-d5	8.11	63	80975	130.15	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	130.15%#
57) 1,1,2,2-Tetrachloroethane-	10.24	84	127196	59.75	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	119.50%
64) 1,2-Dichlorobenzene-d4	11.65	152	149901	77.16	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	154.32%#


Target Compounds					Ovalue
13) Acetone	2.19	43	6911	5.787 ug/L	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071720\
Data File : VV017527.D
Acq On : 17 Jul 2020 15:54
Operator : SY/MD
Sample : L3336-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-1

Quant Time: Jul 18 05:59:42 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jul 18 05:06:25 2020
Response via : Initial Calibration

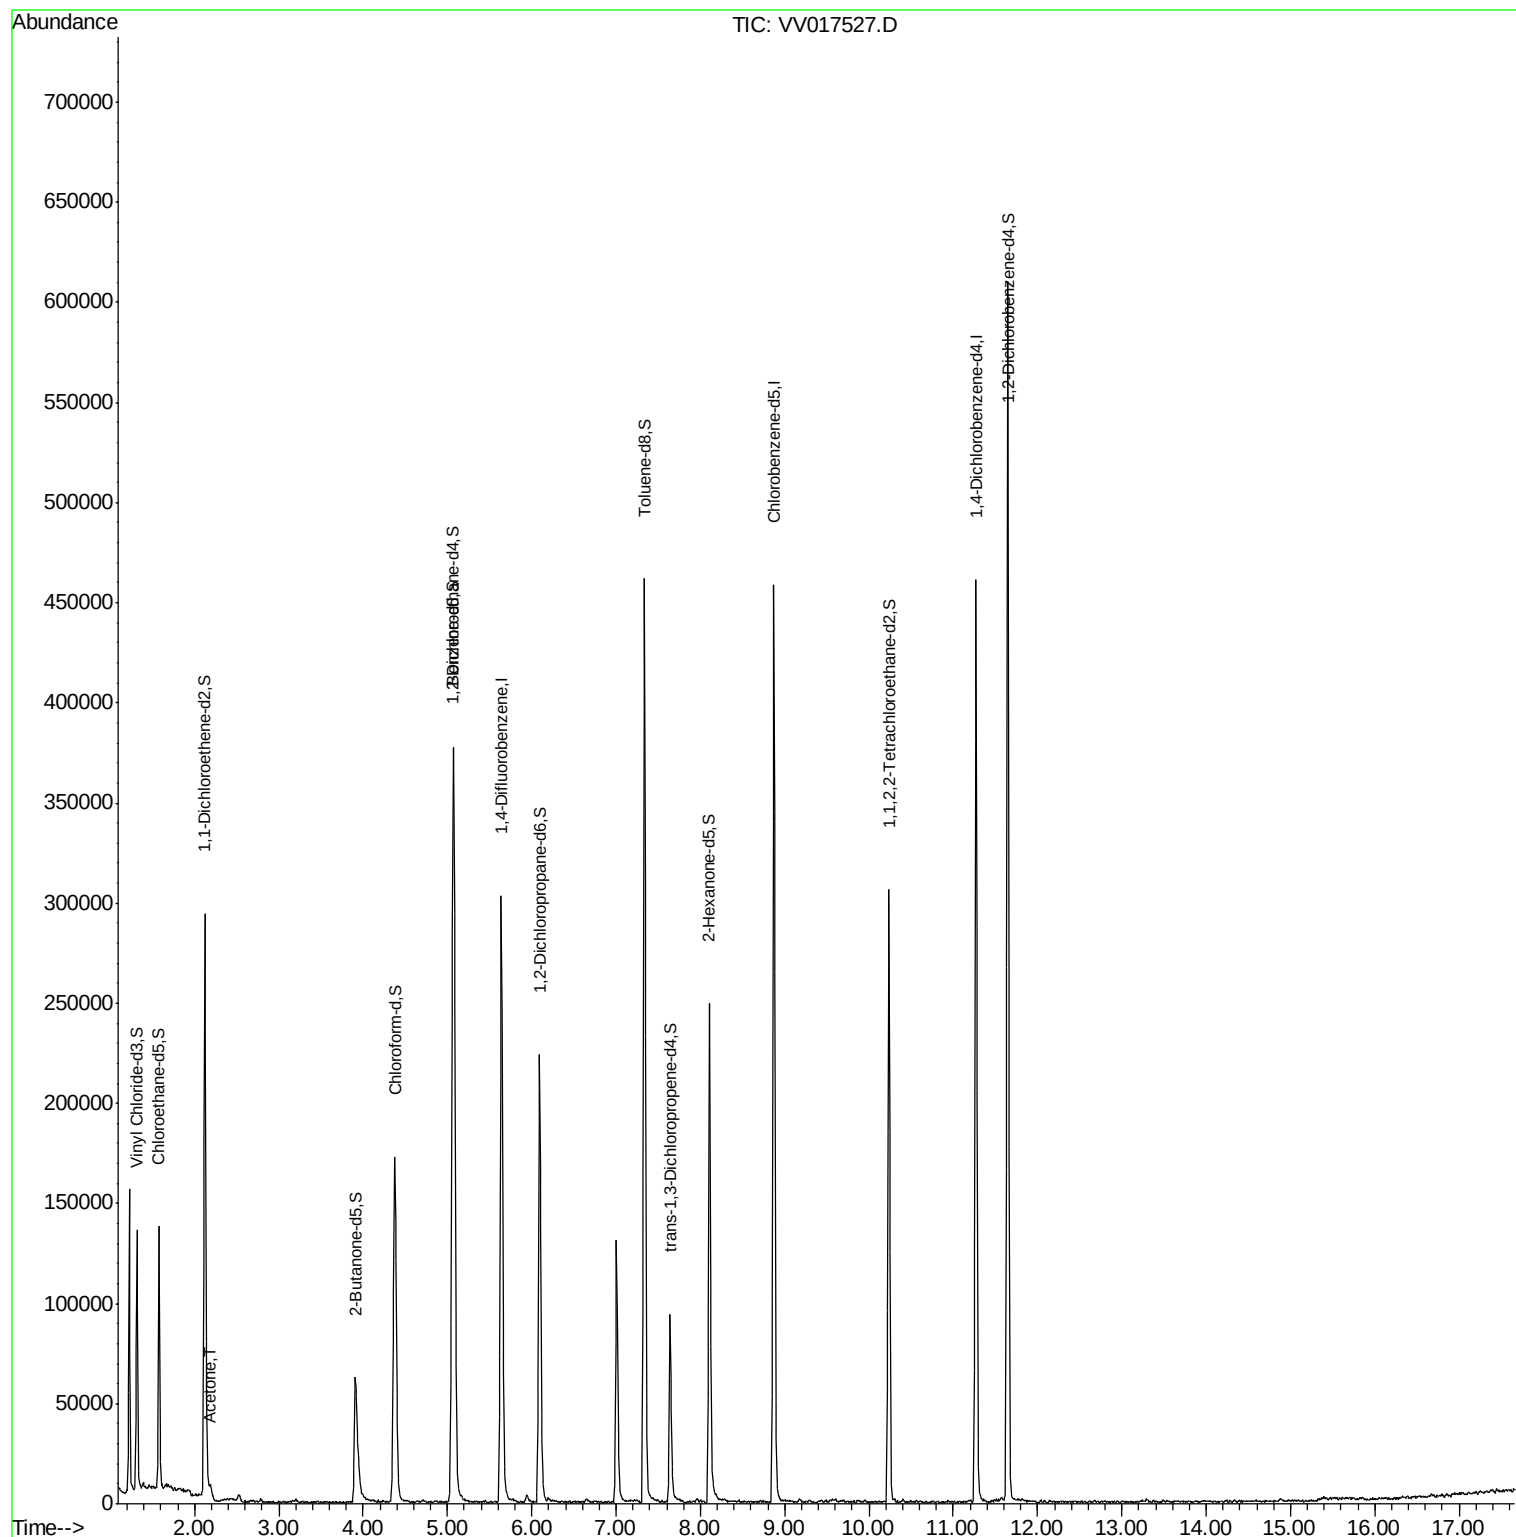

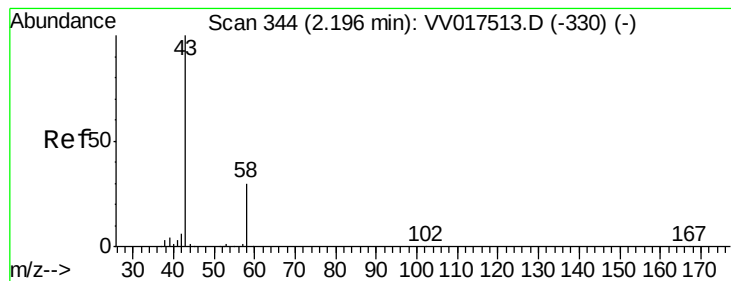

#13
 Acetone
 Concen: 5.787 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. -0.01 min
 Lab File: VV017527.D
 Acq: 17 Jul 2020 15:54

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-1

Tot Ion: 43 Resp: 6911
 Ion Ratio Lower Upper
 43 100
 58 10.8 0.0 56.0

