

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
 Data File : VV071726.D
 Acq On : 17 Jul 2020 15:30
 Operator : SY/MD
 Sample : L3336-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rBV	110995	110109	12.71%	1.395%
2	1.579	146	152	160	rVB	106516	113562	13.11%	1.439%
3	2.123	311	321	337	rBV	254771	382177	44.11%	4.841%
4	2.373	396	399	401	rBV3	730	414	0.05%	0.005%
5	2.782	521	526	538	rVB10	3088	5232	0.60%	0.066%
6	2.907	564	565	569	rBV2	529	390	0.05%	0.005%
7	3.055	609	611	615	rBV2	672	514	0.06%	0.007%
8	3.132	630	635	637	rBV3	508	355	0.04%	0.004%
9	3.145	637	639	642	rVV2	745	383	0.04%	0.005%
10	3.216	647	661	672	rBV5	5174	11990	1.38%	0.152%
11	3.303	686	688	690	rBV2	696	441	0.05%	0.006%
12	3.386	712	714	718	rVB2	760	394	0.05%	0.005%
13	3.428	722	727	730	rBV3	683	610	0.07%	0.008%
14	3.447	730	733	735	rBV2	645	446	0.05%	0.006%
15	3.505	749	751	758	rVV5	1016	865	0.10%	0.011%
16	3.672	800	803	806	rBV2	915	486	0.06%	0.006%
17	3.730	817	821	824	rVV3	649	505	0.06%	0.006%
18	3.936	866	885	910	rBV3	233601	669334	77.25%	8.479%
19	4.222	971	974	977	rBV3	1005	677	0.08%	0.009%
20	4.296	995	997	999	rVB3	946	368	0.04%	0.005%
21	4.376	1007	1022	1045	rBV2	146350	363824	41.99%	4.609%
22	4.521	1064	1067	1070	rBV3	1240	749	0.09%	0.009%
23	4.688	1117	1119	1123	rVB3	638	377	0.04%	0.005%
24	4.740	1131	1135	1138	rBV4	727	483	0.06%	0.006%
25	4.762	1138	1142	1144	rBV2	544	418	0.05%	0.005%
26	4.910	1183	1188	1190	rBV2	1091	863	0.10%	0.011%
27	5.071	1221	1238	1261	rBV2	335599	866458	100.00%	10.976%
28	5.293	1304	1307	1309	rVB3	1097	581	0.07%	0.007%
29	5.483	1363	1366	1369	rBV	698	463	0.05%	0.006%
30	5.544	1379	1385	1388	rVB2	700	659	0.08%	0.008%
31	5.579	1394	1396	1399	rVB3	975	463	0.05%	0.006%
32	5.640	1403	1415	1437	rBV	344116	685065	79.06%	8.678%
33	5.894	1491	1494	1496	rBV2	494	359	0.04%	0.005%
34	5.936	1500	1507	1510	rBV9	2860	3459	0.40%	0.044%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
 Data File : VV017526.D
 Acq On : 17 Jul 2020 15:30
 Operator : SY/MD
 Sample : L3336-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

35	5.991	1521	1524	1527	rBV3	755	561	0.06%	0.007%
36	6.045	1537	1541	1542	rBV3	862	564	0.07%	0.007%
37	6.093	1543	1556	1574	rVV	191799	384256	44.35%	4.868%
38	6.302	1618	1621	1623	rBV3	830	577	0.07%	0.007%
39	6.341	1630	1633	1635	rBV2	803	535	0.06%	0.007%
40	6.376	1641	1644	1645	rBV2	1058	448	0.05%	0.006%
41	6.418	1654	1657	1658	rBV	833	425	0.05%	0.005%
42	6.630	1720	1723	1724	rBV3	540	354	0.04%	0.004%
43	6.646	1726	1728	1730	rBV2	885	455	0.05%	0.006%
44	6.733	1752	1755	1757	rBV3	578	454	0.05%	0.006%
45	6.769	1763	1766	1768	rBV2	682	358	0.04%	0.005%
46	6.878	1796	1800	1804	rBV4	501	517	0.06%	0.007%
47	7.007	1829	1840	1862	rBV	114141	206115	23.79%	2.611%
48	7.142	1880	1882	1886	rBV3	884	521	0.06%	0.007%
49	7.280	1923	1925	1930	rVB3	1002	563	0.06%	0.007%
50	7.338	1930	1943	1962	rBV	399613	692693	79.95%	8.775%
51	7.643	2027	2038	2059	rBV	91329	168085	19.40%	2.129%
52	7.872	2107	2109	2111	rBV2	1063	490	0.06%	0.006%
53	7.958	2133	2136	2137	rBV3	1782	1063	0.12%	0.013%
54	8.048	2158	2164	2165	rBV3	1077	914	0.11%	0.012%
55	8.106	2172	2182	2205	rBV	242546	431271	49.77%	5.463%
56	8.608	2336	2338	2340	rVV3	1200	457	0.05%	0.006%
57	8.646	2347	2350	2352	rBV3	864	560	0.06%	0.007%
58	8.871	2409	2420	2440	rBV	513668	828866	95.66%	10.500%
59	9.000	2458	2460	2463	rBV3	827	608	0.07%	0.008%
60	9.177	2513	2515	2519	rBV2	596	354	0.04%	0.004%
61	9.261	2539	2541	2546	rVV3	632	428	0.05%	0.005%
62	9.338	2562	2565	2570	rVV5	556	579	0.07%	0.007%
63	9.373	2574	2576	2580	rVV	789	475	0.05%	0.006%
64	9.444	2595	2598	2601	rBV3	887	634	0.07%	0.008%
65	9.608	2646	2649	2653	rBV4	618	499	0.06%	0.006%
66	9.698	2674	2677	2682	rBV3	1139	820	0.09%	0.010%
67	9.852	2721	2725	2727	rBV2	835	660	0.08%	0.008%
68	10.154	2815	2819	2822	rBV3	557	463	0.05%	0.006%
69	10.238	2833	2845	2859	rBV	265479	423281	48.85%	5.362%
70	10.328	2871	2873	2875	rBV2	929	565	0.07%	0.007%
71	10.482	2919	2921	2924	rBV2	623	417	0.05%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
 Data File : VV071726.D
 Acq On : 17 Jul 2020 15:30
 Operator : SY/MD
 Sample : L3336-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

72	10.534	2934	2937	2942	rVB4	1009	558	0.06%	0.007%
73	10.704	2988	2990	2993	rBV2	1039	619	0.07%	0.008%
74	10.743	3000	3002	3005	rBV4	641	407	0.05%	0.005%
75	10.820	3022	3026	3029	rBV3	748	389	0.04%	0.005%
76	10.871	3038	3042	3046	rBV5	844	922	0.11%	0.012%
77	11.084	3105	3108	3114	rVB4	1015	974	0.11%	0.012%
78	11.270	3153	3166	3184	rBV	517601	803276	92.71%	10.176%
79	11.566	3250	3258	3264	rBV8	1594	2311	0.27%	0.029%
80	11.646	3271	3283	3304	rBV	448253	697386	80.49%	8.834%
81	11.762	3316	3319	3324	rVB5	1173	1157	0.13%	0.015%
82	11.887	3355	3358	3362	rBV3	569	470	0.05%	0.006%
83	12.039	3403	3405	3407	rBV	793	430	0.05%	0.005%
84	12.077	3415	3417	3420	rBV3	719	444	0.05%	0.006%
85	12.225	3460	3463	3465	rBV3	773	364	0.04%	0.005%
86	12.293	3482	3484	3488	rVB3	591	392	0.05%	0.005%
87	12.752	3625	3627	3629	rBV	722	380	0.04%	0.005%
88	12.993	3700	3702	3704	rBV	783	508	0.06%	0.006%
89	13.090	3727	3732	3735	rVB2	566	511	0.06%	0.006%
90	13.132	3743	3745	3750	rVB3	624	455	0.05%	0.006%
91	13.235	3771	3777	3779	rBV3	1119	1175	0.14%	0.015%
92	13.289	3789	3794	3795	rBV3	2639	2540	0.29%	0.032%
93	13.575	3882	3883	3885	rBV2	1042	491	0.06%	0.006%
94	13.720	3926	3928	3930	rBV2	951	372	0.04%	0.005%
95	13.823	3957	3960	3961	rBV3	945	667	0.08%	0.008%
96	14.456	4153	4157	4160	rBV4	1108	841	0.10%	0.011%
97	14.505	4168	4172	4173	rBV2	583	383	0.04%	0.005%
98	14.675	4223	4225	4228	rBV2	885	405	0.05%	0.005%
99	14.820	4267	4270	4274	rBV3	621	474	0.05%	0.006%
100	15.199	4386	4388	4390	rBV3	986	494	0.06%	0.006%


Sum of corrected areas: 7894153

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071720\
Data File : VV071726.D
Acq On : 17 Jul 2020 15:30
Operator : SY/MD
Sample : L3336-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

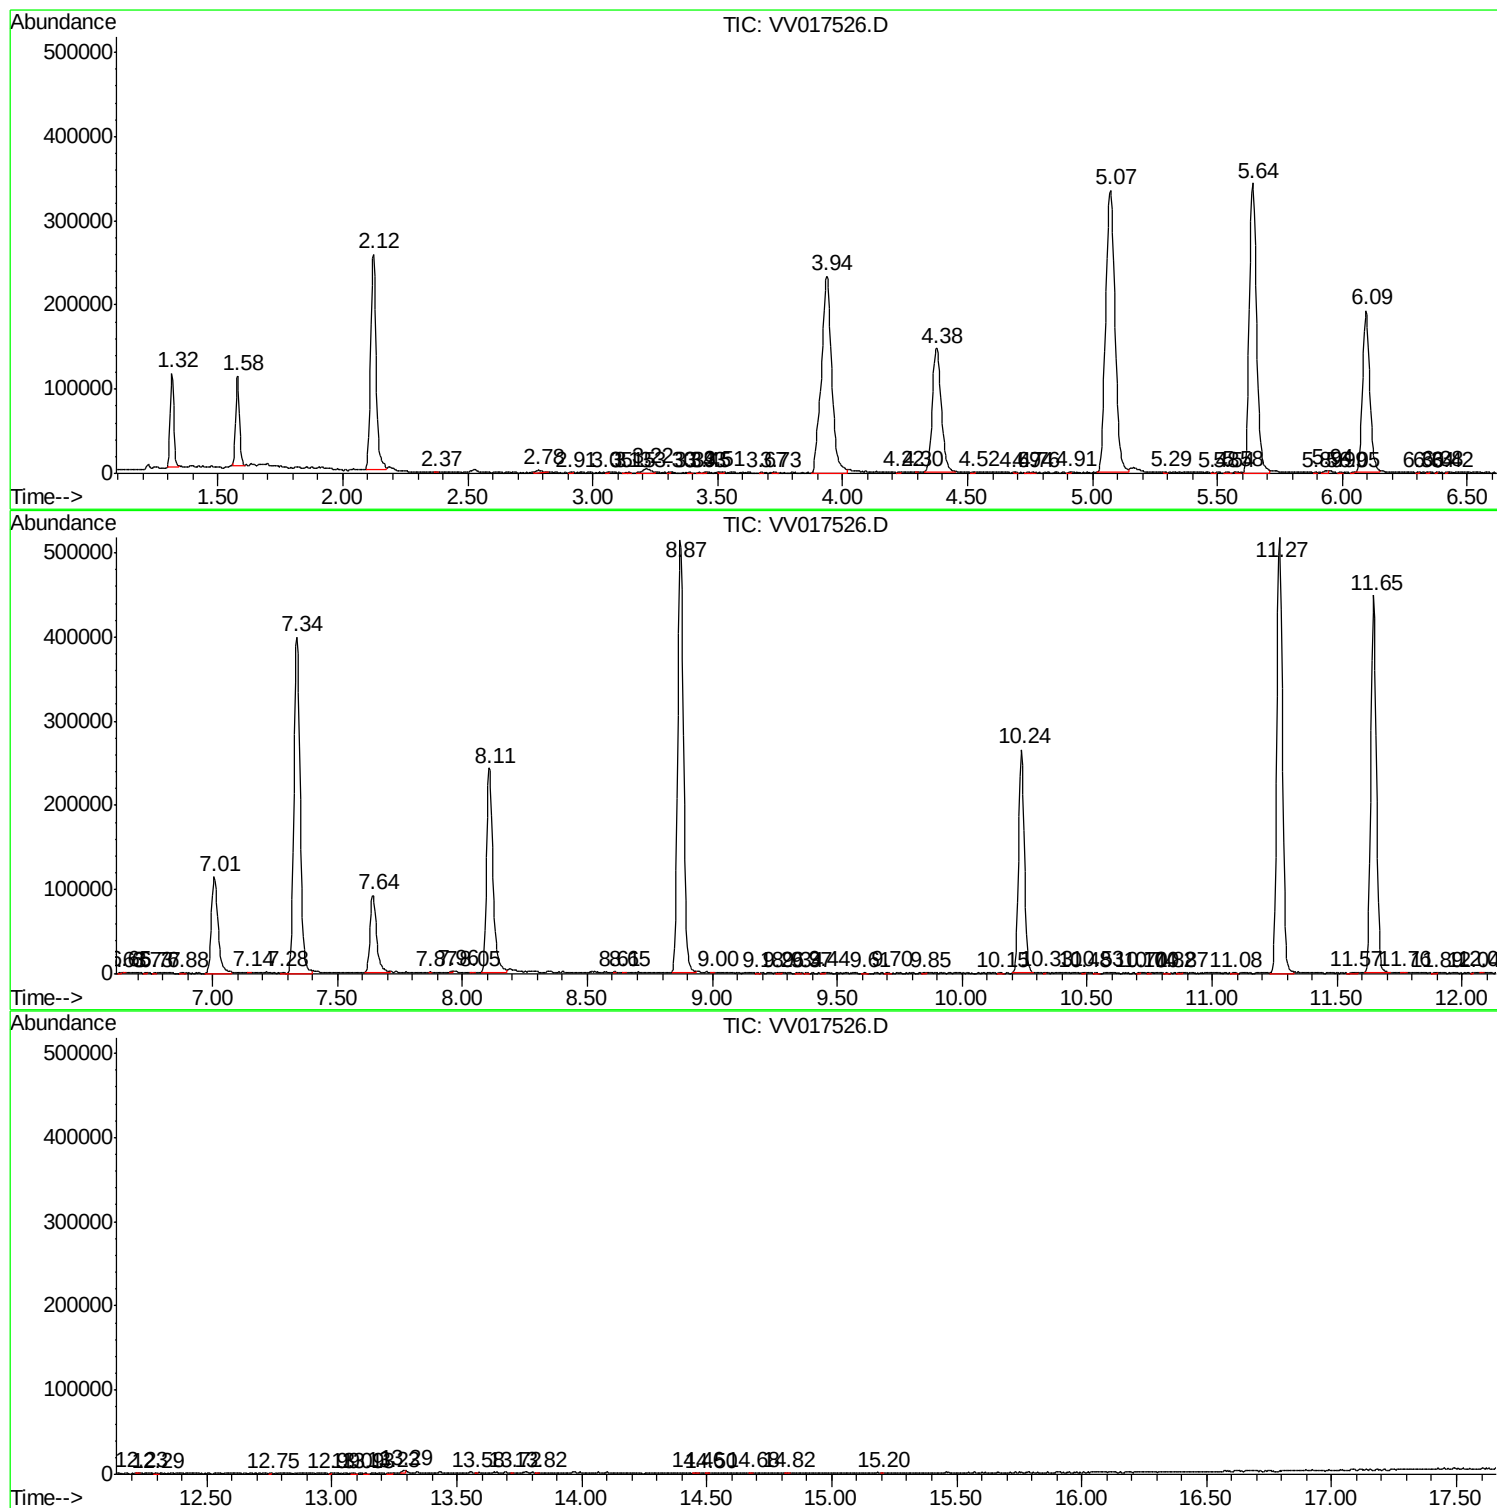

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV071720\
Data File : VV017526.D
Acq On : 17 Jul 2020 15:30
Operator : SY/MD
Sample : L3336-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071720\
Data File : VV017526.D
Acq On : 17 Jul 2020 15:30
Operator : SY/MD
Sample : L3336-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc