

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
 Data File : VV0717531.D
 Acq On : 17 Jul 2020 18:13
 Operator : SY/MD
 Sample : L3336-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	65	70	81	rVB	114359	116364	1.23%	0.332%
2	1.579	146	152	164	rVB	116510	127669	1.35%	0.364%
3	2.123	312	321	338	rBV	262782	394260	4.17%	1.123%
4	2.701	496	501	503	rBV3	598	556	0.01%	0.002%
5	3.026	600	602	603	rBV	605	308	0.00%	0.001%
6	3.087	618	621	623	rVV2	647	326	0.00%	0.001%
7	3.103	623	626	629	rVB3	837	567	0.01%	0.002%
8	3.161	643	644	646	rBV	507	283	0.00%	0.001%
9	3.190	652	653	656	rBV2	476	240	0.00%	0.001%
10	3.203	656	657	659	rBV2	830	369	0.00%	0.001%
11	3.357	703	705	707	rBV	538	232	0.00%	0.001%
12	3.367	707	708	711	rVB3	783	283	0.00%	0.001%
13	3.489	744	746	748	rBV2	929	483	0.01%	0.001%
14	3.502	748	750	753	rVV4	516	264	0.00%	0.001%
15	3.560	765	768	769	rBV3	912	468	0.00%	0.001%
16	3.759	827	830	832	rBV3	689	530	0.01%	0.002%
17	3.913	867	878	912	rBV2	86300	286336	3.03%	0.816%
18	4.377	1007	1022	1049	rBV2	189013	449192	4.75%	1.280%
19	4.669	1109	1113	1116	rBV5	1096	798	0.01%	0.002%
20	4.688	1117	1119	1123	rBV4	976	667	0.01%	0.002%
21	4.868	1172	1175	1177	rBV2	1104	799	0.01%	0.002%
22	4.910	1186	1188	1191	rBV3	558	357	0.00%	0.001%
23	4.923	1191	1192	1198	rVB3	905	795	0.01%	0.002%
24	5.071	1221	1238	1251	rBV3	399079	1038740	10.99%	2.959%
25	5.351	1322	1325	1327	rBV3	1357	712	0.01%	0.002%
26	5.495	1367	1370	1373	rBV3	848	656	0.01%	0.002%
27	5.582	1392	1397	1398	rBV3	1449	1046	0.01%	0.003%
28	5.640	1403	1415	1435	rVV	436476	847820	8.97%	2.416%
29	5.830	1472	1474	1476	rBV3	827	334	0.00%	0.001%
30	5.942	1498	1509	1527	rBV3	40734	83310	0.88%	0.237%
31	6.093	1544	1556	1574	rBV	222611	442486	4.68%	1.261%
32	6.232	1596	1599	1603	rBV3	1144	859	0.01%	0.002%
33	6.274	1610	1612	1615	rBV2	720	367	0.00%	0.001%
34	6.312	1622	1624	1627	rBV2	422	301	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
 Data File : VV0717531.D
 Acq On : 17 Jul 2020 18:13
 Operator : SY/MD
 Sample : L3336-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

35	6.373	1640	1643	1645	rBV2	796	533	0.01%	0.002%
36	6.386	1645	1647	1651	rVB3	672	399	0.00%	0.001%
37	6.431	1659	1661	1666	rVB4	977	541	0.01%	0.002%
38	6.450	1666	1667	1670	rVB3	601	225	0.00%	0.001%
39	6.521	1686	1689	1692	rBV3	1001	649	0.01%	0.002%
40	6.634	1722	1724	1725	rBV	693	350	0.00%	0.001%
41	6.708	1745	1747	1749	rBV3	524	243	0.00%	0.001%
42	6.769	1761	1766	1768	rVB	475	400	0.00%	0.001%
43	6.788	1769	1772	1773	rVV	484	233	0.00%	0.001%
44	6.929	1812	1816	1818	rBV3	603	557	0.01%	0.002%
45	6.952	1820	1823	1826	rVB3	772	616	0.01%	0.002%
46	7.007	1829	1840	1858	rBV	123150	223421	2.36%	0.637%
47	7.338	1931	1943	1956	rBV	432214	743951	7.87%	2.120%
48	7.412	1957	1966	1987	rVB	116321	207712	2.20%	0.592%
49	7.640	2027	2037	2055	rBV	90721	158124	1.67%	0.451%
50	7.823	2093	2094	2098	rVB3	639	295	0.00%	0.001%
51	7.843	2098	2100	2102	rBV3	666	301	0.00%	0.001%
52	7.997	2137	2148	2166	rVB2	109015	182761	1.93%	0.521%
53	8.106	2173	2182	2199	rBV	253911	425280	4.50%	1.212%
54	8.531	2312	2314	2315	rBV	574	275	0.00%	0.001%
55	8.550	2318	2320	2325	rBV3	835	699	0.01%	0.002%
56	8.646	2346	2350	2351	rBV2	532	307	0.00%	0.001%
57	8.656	2351	2353	2357	rVB3	496	259	0.00%	0.001%
58	8.679	2357	2360	2363	rBV3	919	636	0.01%	0.002%
59	8.701	2366	2367	2370	rVV3	744	423	0.00%	0.001%
60	8.730	2374	2376	2379	rVV2	474	250	0.00%	0.001%
61	8.765	2383	2387	2389	rVV2	1048	703	0.01%	0.002%
62	8.788	2392	2394	2396	rVB2	904	430	0.00%	0.001%
63	8.804	2396	2399	2402	rBV3	917	471	0.00%	0.001%
64	8.904	2409	2430	2451	rBV2	4206253	7686207	81.30%	21.899%
65	9.273	2543	2545	2547	rBV2	655	280	0.00%	0.001%
66	9.457	2601	2602	2605	rVB3	804	401	0.00%	0.001%
67	9.569	2625	2637	2648	rBV4	5819	10440	0.11%	0.030%
68	9.611	2648	2650	2655	rBV3	954	395	0.00%	0.001%
69	9.691	2673	2675	2679	rBV3	959	713	0.01%	0.002%
70	9.888	2733	2736	2738	rBV2	1050	625	0.01%	0.002%
71	9.939	2748	2752	2754	rBV2	1015	962	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071720\
 Data File : VV017531.D
 Acq On : 17 Jul 2020 18:13
 Operator : SY/MD
 Sample : L3336-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 PMW-6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis

72	9.994	2764	2769	2771	rBV3	999	876	0.01%	0.002%
73	10.074	2792	2794	2796	rBV2	693	306	0.00%	0.001%
74	10.103	2799	2803	2804	rBV2	840	635	0.01%	0.002%
75	10.129	2809	2811	2812	rBV2	754	240	0.00%	0.001%
76	10.238	2834	2845	2863	rVB	324160	513742	5.43%	1.464%
77	10.344	2876	2878	2881	rBV3	1030	636	0.01%	0.002%
78	10.466	2912	2916	2917	rBV	1684	1215	0.01%	0.003%
79	10.547	2939	2941	2943	rBV3	1210	631	0.01%	0.002%
80	10.672	2978	2980	2982	rBV	579	261	0.00%	0.001%
81	10.720	2990	2995	2999	rBV5	844	984	0.01%	0.003%
82	10.736	2999	3000	3003	rVV3	636	295	0.00%	0.001%
83	10.794	3016	3018	3020	rBV	605	363	0.00%	0.001%
84	11.064	3099	3102	3106	rBV2	517	446	0.00%	0.001%
85	11.080	3106	3107	3109	rBV2	828	321	0.00%	0.001%
86	11.203	3133	3145	3157	rBV	2291432	3472953	36.74%	9.895%
87	11.293	3157	3173	3198	rVB2	5661048	9453855	100.00%	26.935%
88	11.656	3271	3286	3305	rBV2	789483	1832019	19.38%	5.220%
89	11.862	3340	3350	3357	rBV10	3440	6334	0.07%	0.018%
90	12.280	3474	3480	3484	rVB8	1297	1380	0.01%	0.004%
91	12.434	3525	3528	3529	rBV2	1240	656	0.01%	0.002%
92	12.521	3552	3555	3557	rBV2	1100	712	0.01%	0.002%
93	12.672	3594	3602	3609	rBV5	10083	15546	0.16%	0.044%
94	12.813	3644	3646	3649	rBV3	1461	965	0.01%	0.003%
95	12.858	3657	3660	3664	rBV3	857	654	0.01%	0.002%
96	13.170	3754	3757	3762	rBV6	1021	620	0.01%	0.002%
97	13.283	3779	3792	3812	rBV	3939013	5876716	62.16%	16.743%
98	13.765	3932	3942	3958	rVB	293344	464135	4.91%	1.322%
99	15.045	4339	4340	4343	rBV	900	564	0.01%	0.002%
100	15.093	4353	4355	4358	rBV4	1389	715	0.01%	0.002%


Sum of corrected areas: 35098619

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071720\
Data File : VV017531.D
Acq On : 17 Jul 2020 18:13
Operator : SY/MD
Sample : L3336-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

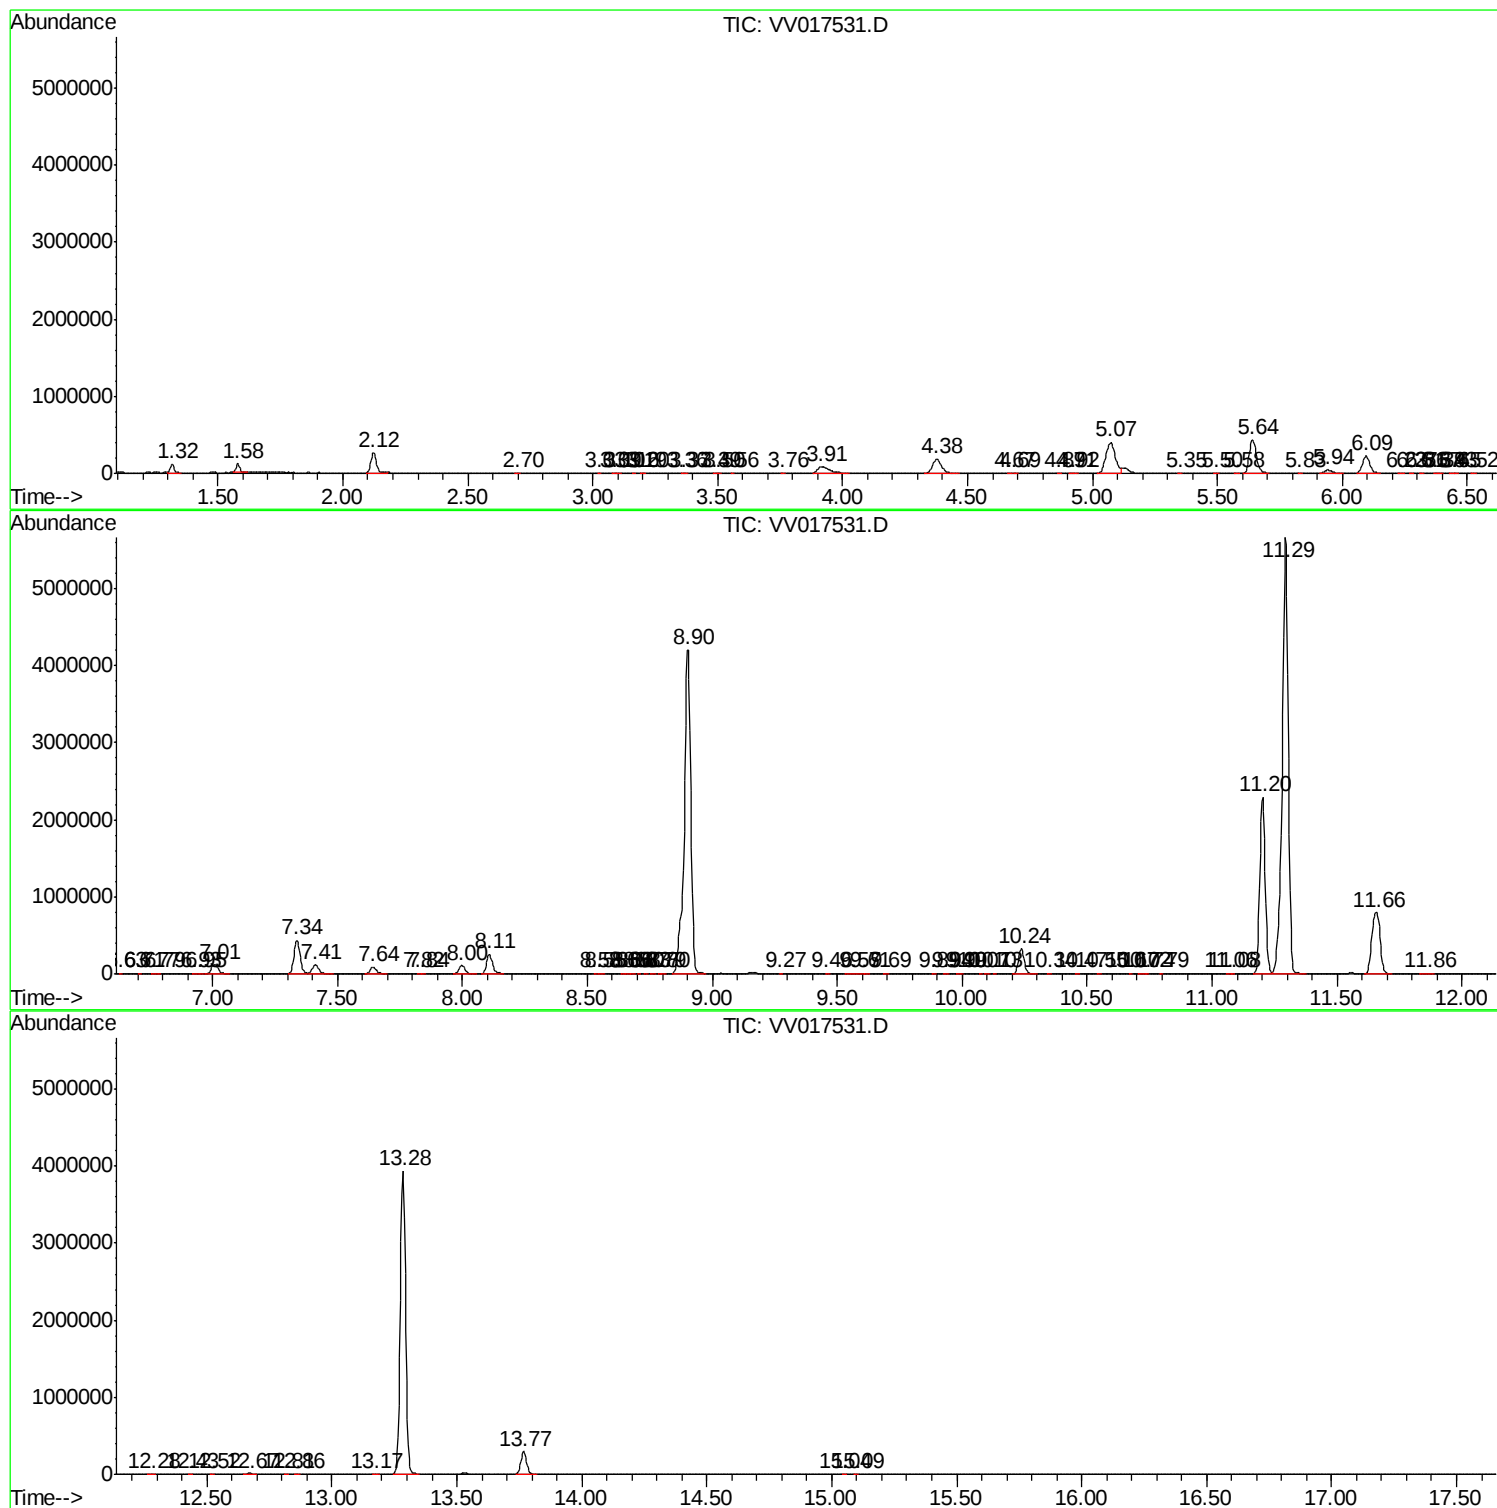

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071720\
Data File : VV017531.D
Acq On : 17 Jul 2020 18:13
Operator : SY/MD
Sample : L3336-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071720\
Data File : VV017531.D
Acq On : 17 Jul 2020 18:13
Operator : SY/MD
Sample : L3336-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
PMW-6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc