


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV071720\
 Data File : VV017512.D
 Acq On : 17 Jul 2020 08:37
 Operator : SY/MD
 Sample : BFB62
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM070820WMA.M
 Title : VOC Analysis
 Last Update : Sat Jul 18 05:06:25 2020

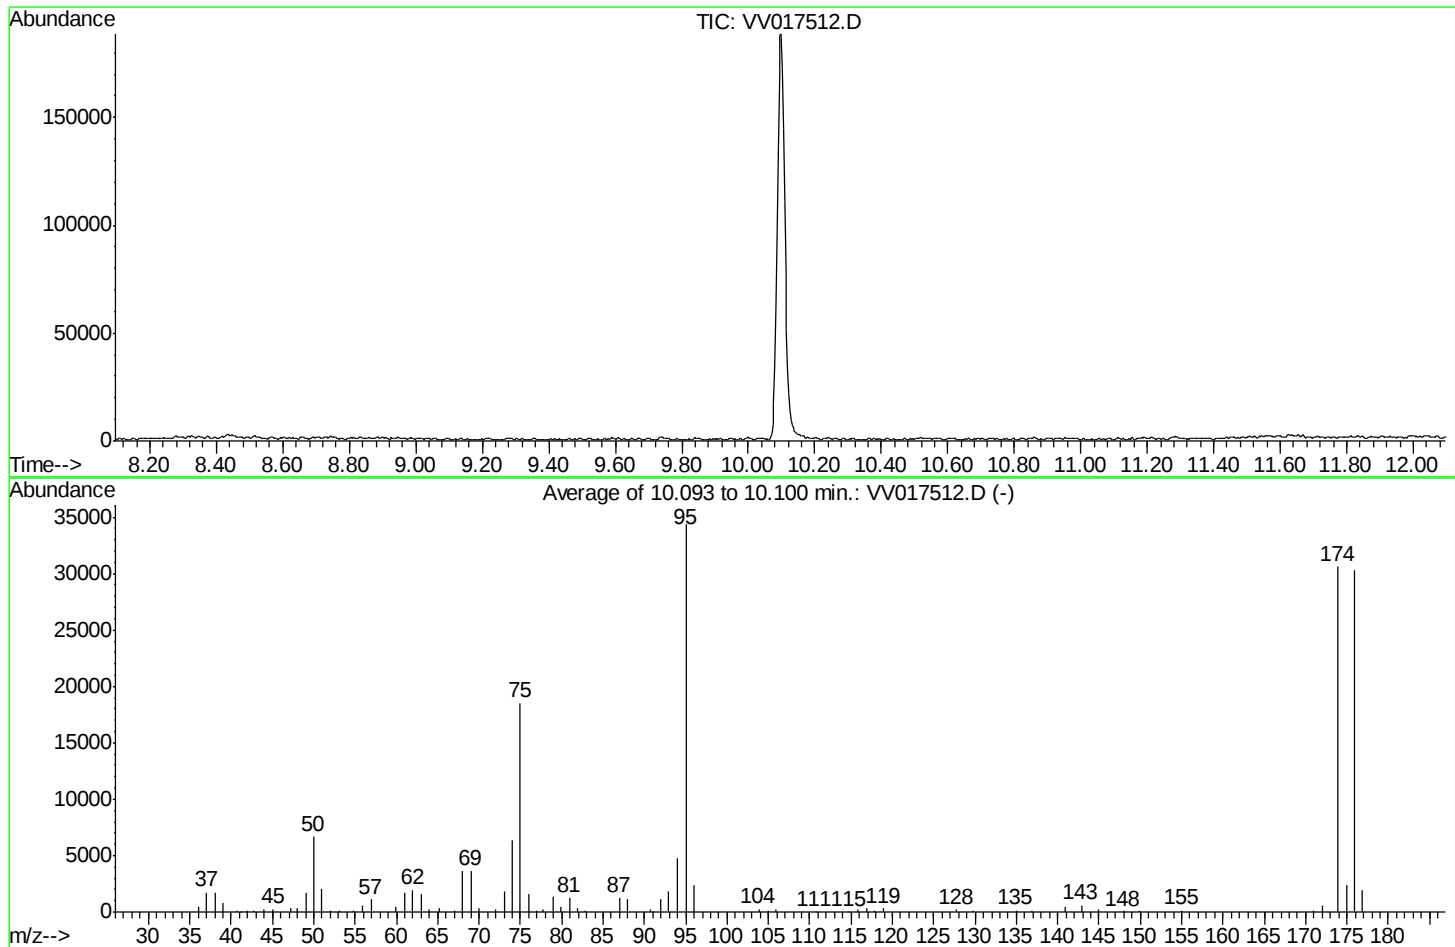

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	6661	PASS
75	95	30	80	53.9	18530	PASS
95	95	100	100	100.0	34365	PASS
96	95	5	9	7.0	2392	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.1	30621	PASS
175	174	5	9	7.7	2371	PASS
176	174	95	101	98.8	30256	PASS
177	176	5	9	6.3	1897	PASS

m/z	Abundance
36.00	380.0
37.00	1807.0
38.00	1550.0
39.00	675.0
39.90	205.0
40.70	145.0
42.00	142.0
42.70	121.0
43.90	487.0
45.10	256.0
47.20	227.0
48.00	296.0
49.00	1626.0
50.00	6527.0
51.00	2024.0
52.00	165.0
54.80	120.0
55.90	576.0
56.90	1118.0
59.90	383.0
60.90	1642.0
62.00	1718.0
63.00	1518.0
64.00	208.0
65.10	360.0
67.10	161.0
68.00	3526.0
69.00	3636.0
69.90	311.0
72.00	226.0
73.00	1526.0
74.00	6096.0
75.00	17560.0
76.00	1428.0
77.00	165.0
77.70	245.0
78.90	1264.0
79.90	367.0
80.90	1214.0
81.90	273.0
86.90	1221.0
88.00	1162.0
90.70	230.0
92.00	1154.0
92.90	1556.0
94.00	4673.0
95.00	32008.0
96.00	2285.0
103.90	236.0
105.10	156.0
105.90	158.0
114.80	121.0
115.70	291.0
116.90	296.0
117.80	176.0
119.00	246.0
127.80	152.0
129.80	185.0
134.90	153.0
136.90	130.0
140.90	457.0
142.90	656.0
145.00	240.0
148.00	120.0
149.90	107.0
172.20	534.0
173.90	27696.0
175.00	2160.0
175.90	26744.0
176.90	1902.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	447.0
37.10	1798.0
38.00	1683.0
39.00	749.0
40.00	219.0
40.70	113.0
42.00	131.0
42.60	104.0
44.00	434.0
45.10	300.0
47.20	302.0
48.00	359.0
49.00	1733.0
50.00	6839.0
51.00	2149.0
52.00	174.0
53.20	101.0
54.80	145.0
55.90	565.0
56.90	1144.0
60.00	448.0
60.90	1779.0
62.00	1991.0
63.00	1658.0
63.90	269.0
65.10	387.0
67.10	170.0
68.00	3757.0
69.00	3730.0
69.90	314.0
71.90	227.0
73.00	1826.0
74.00	6680.0
75.00	19192.0
76.00	1593.0
77.00	154.0
77.70	229.0
78.90	1336.0
79.90	405.0
80.90	1343.0
81.90	341.0
82.80	124.0
86.90	1312.0
87.90	1194.0
90.70	227.0
92.00	1138.0
92.90	1870.0
94.00	4903.0
95.00	35584.0
96.00	2488.0
103.90	244.0
105.10	151.0
105.90	232.0
115.70	284.0
116.90	309.0
117.90	181.0
118.90	328.0
127.80	184.0
129.80	164.0
135.00	169.0
136.90	141.0
141.00	497.0
142.90	633.0
145.00	244.0
148.00	123.0
149.90	115.0
155.00	146.0
170.90	129.0
172.10	546.0
173.90	31512.0
175.00	2419.0
175.90	31288.0
176.90	1940.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	434.0
37.00	1644.0
38.00	1719.0
39.00	837.0
40.00	224.0
41.20	100.0
42.00	112.0
44.00	359.0
45.10	278.0
47.20	348.0
47.90	333.0
49.00	1654.0
50.00	6618.0
51.00	2023.0
52.10	167.0
53.10	130.0
54.90	178.0
56.00	568.0
57.00	1059.0
59.90	451.0
61.00	1788.0
62.00	2104.0
63.00	1581.0
64.00	315.0
65.10	380.0
67.10	137.0
68.00	3741.0
69.00	3693.0
69.90	301.0
71.90	240.0
73.00	1968.0
74.00	6425.0
75.00	18840.0
76.00	1592.0
76.90	148.0
77.70	170.0
78.90	1411.0
79.80	438.0
80.90	1213.0
81.90	413.0
82.80	127.0
87.00	1258.0
87.90	1097.0
90.70	156.0
91.00	122.0
92.00	1024.0
92.90	2060.0
94.00	4622.0
95.00	35504.0
96.00	2403.0
103.80	243.0
105.00	108.0
105.90	243.0
110.70	137.0
115.80	212.0
116.90	284.0
118.00	143.0
118.90	337.0
127.80	196.0
129.80	125.0
135.10	150.0
136.90	125.0
141.00	496.0
142.90	566.0
145.00	197.0
155.00	216.0
171.00	129.0
172.00	529.0
174.00	32656.0
175.00	2534.0
175.90	32736.0
176.90	1850.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

Scan 2790 (10.061 min): VV017512.D
BFB62

m/z	Abundance
39.80	218.0
43.90	232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62