
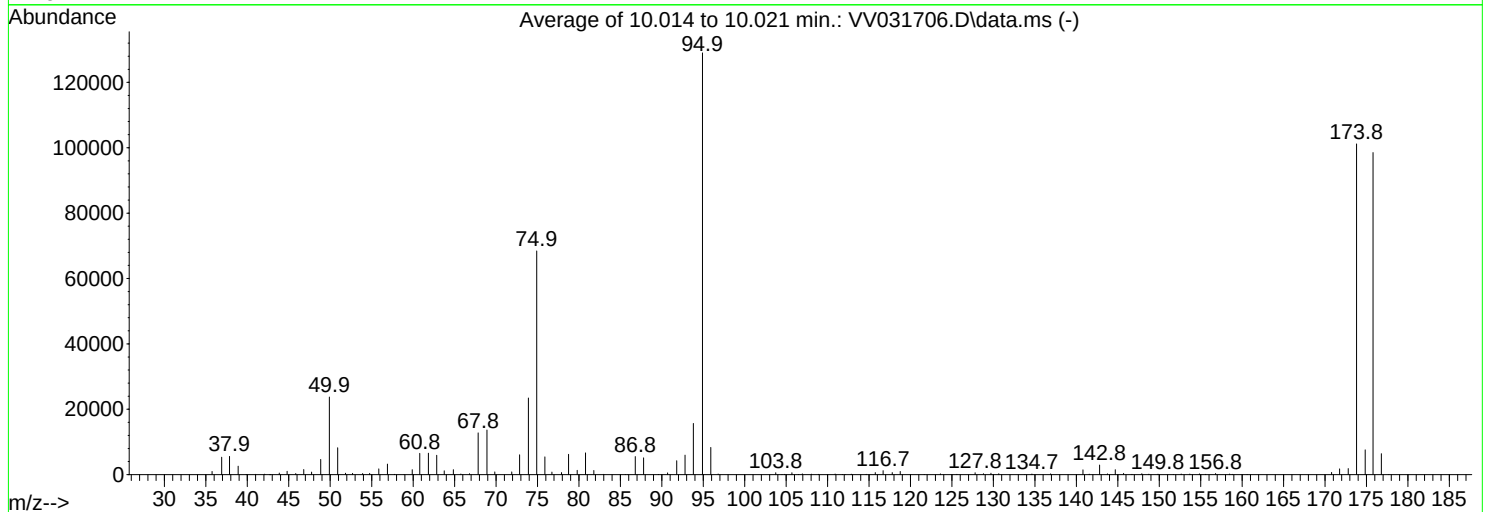


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071723\
Data File : VV031706.D
Acq On : 17 Jul 2023 08:52
Operator : SY/MD
Sample : BFB283
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB283

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Jul 18 06:24:32 2023

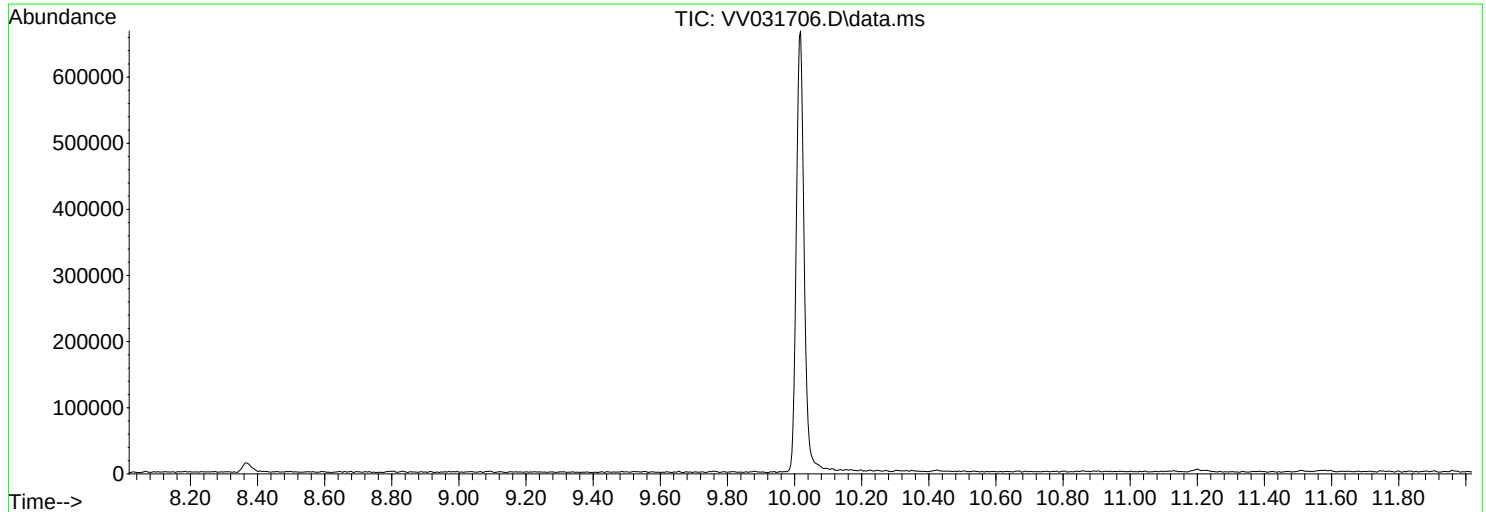

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	23720	PASS
75	95	30	80	53.0	68443	PASS
95	95	100	100	100.0	129029	PASS
96	95	5	9	6.4	8306	PASS
173	174	0.00	2	1.8	1862	PASS
174	95	50	120	78.4	101171	PASS
175	174	5	9	7.5	7575	PASS
176	174	95	105	97.4	98509	PASS
177	176	5	10	6.5	6406	PASS

m/z	Abundance
35.60	205.0
36.60	118.0
37.30	131.0
38.10	171.0
39.80	496.0
42.70	148.0
43.80	877.0
45.00	105.0
46.00	114.0
47.00	139.0
50.20	167.0
53.00	245.0
57.30	153.0
60.20	104.0
63.70	108.0
78.70	129.0
110.00	113.0
136.60	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
35.80	1252.0
36.90	5406.0
37.80	5955.0
38.90	2846.0
40.00	654.0
41.00	124.0
42.10	219.0
42.80	131.0
43.90	1519.0
44.80	1261.0
45.80	499.0
46.80	1713.0
47.80	836.0
48.90	4724.0
49.90	25272.0
50.90	8351.0
51.90	421.0
52.80	377.0
53.90	346.0
54.90	351.0
55.90	1906.0
56.90	3359.0
57.70	100.0
58.90	114.0
59.90	1534.0
60.80	6488.0
61.90	6700.0
62.80	6096.0
63.80	1417.0
64.90	1447.0
65.80	198.0
66.80	395.0
67.80	13131.0
68.90	14083.0
69.90	941.0
71.90	919.0
72.90	6389.0
73.90	24616.0
74.90	70584.0
75.90	5519.0
76.80	801.0
77.90	677.0
78.80	6458.0
79.80	1435.0
80.80	6694.0
81.80	1269.0
83.00	100.0
85.60	195.0
86.80	5612.0
87.80	5320.0
89.60	103.0
90.70	514.0
91.80	4330.0
92.80	6332.0
93.80	15701.0
94.90	132224.0
95.90	9171.0
96.80	214.0
103.70	581.0
104.50	211.0
105.70	654.0
106.90	269.0
108.00	137.0
110.90	197.0
111.80	100.0
112.80	138.0
114.70	129.0
115.80	659.0
116.70	1385.0
117.80	680.0
118.70	1081.0
121.70	116.0
123.60	229.0
127.80	596.0
128.80	243.0
129.70	554.0
130.70	352.0
134.70	241.0
136.80	278.0
140.80	1503.0
141.60	232.0
142.80	3052.0
143.80	237.0
144.70	1578.0
145.70	376.0
146.70	130.0
147.90	364.0
148.70	147.0
149.80	164.0
152.60	197.0
153.70	180.0
154.90	260.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

156.80	323.0
158.50	184.0
158.80	185.0
160.60	117.0
170.80	577.0
171.80	1705.0
172.70	1705.0
173.80	100832.0
174.80	8074.0
175.80	98600.0
176.80	6530.0
177.70	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
35.80	1251.0
36.90	5506.0
37.90	5897.0
38.90	2676.0
39.90	553.0
41.00	120.0
42.10	185.0
42.70	155.0
43.90	1415.0
44.80	1136.0
45.90	469.0
46.80	1754.0
47.70	837.0
48.80	4809.0
49.90	24552.0
50.90	8670.0
51.80	451.0
52.70	363.0
53.90	369.0
54.70	387.0
55.80	1762.0
56.90	3460.0
57.70	112.0
58.90	105.0
59.90	1564.0
60.80	6776.0
61.80	6742.0
62.90	6042.0
63.80	1300.0
64.90	1531.0
65.70	206.0
66.80	295.0
67.90	13195.0
68.90	14144.0
69.90	861.0
71.90	858.0
72.90	6258.0
73.90	24456.0
74.90	70848.0
75.90	5561.0
76.80	798.0
77.90	677.0
78.80	6469.0
79.80	1382.0
80.80	6797.0
81.80	1352.0
83.00	108.0
86.80	5681.0
87.80	5244.0
90.70	561.0
91.80	4406.0
92.80	6225.0
93.80	16284.0
94.90	133376.0
95.90	8532.0
96.80	215.0
103.70	639.0
104.80	178.0
105.70	596.0
106.90	297.0
108.10	165.0
108.90	151.0
110.90	212.0
112.80	171.0
114.60	121.0
115.80	686.0
116.70	1274.0
117.80	669.0
118.80	1008.0
121.60	105.0
123.60	281.0
125.60	122.0
127.80	637.0
128.80	298.0
129.70	482.0
130.60	303.0
134.70	223.0
136.90	226.0
140.80	1567.0
141.50	201.0
142.80	3069.0
143.70	292.0
144.70	1642.0
145.70	389.0
146.70	119.0
147.90	311.0
148.70	155.0
149.90	147.0
152.60	238.0
153.70	207.0
154.80	247.0
155.60	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

156.80	350.0
158.50	228.0
158.80	195.0
170.80	731.0
171.70	1837.0
172.80	1820.0
173.80	104760.0
174.80	7810.0
175.80	101880.0
176.80	6660.0
177.70	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

m/z	Abundance
35.80	1130.0
36.90	5116.0
37.90	4963.0
38.90	2333.0
39.80	492.0
42.00	120.0
42.70	172.0
43.90	1249.0
44.80	963.0
45.90	455.0
46.80	1622.0
47.70	764.0
48.80	4456.0
49.90	21336.0
50.90	7645.0
51.80	510.0
52.60	400.0
53.90	405.0
54.70	422.0
55.80	1661.0
56.90	2964.0
57.80	128.0
59.90	1495.0
60.80	6261.0
61.80	6228.0
62.90	5654.0
63.80	1218.0
64.80	1598.0
65.70	237.0
66.70	183.0
67.90	12049.0
68.90	12779.0
69.80	740.0
71.90	765.0
72.80	5552.0
73.90	21336.0
74.90	63896.0
75.90	5190.0
76.70	767.0
77.90	594.0
78.80	6073.0
79.80	1159.0
80.80	6544.0
81.80	1198.0
83.00	128.0
85.90	214.0
86.80	5311.0
87.80	4911.0
90.70	564.0
91.80	4043.0
92.80	5361.0
93.80	15075.0
94.90	121488.0
95.90	7215.0
96.80	203.0
103.80	577.0
104.80	147.0
105.70	467.0
106.50	212.0
107.00	212.0
108.00	170.0
108.90	142.0
110.90	166.0
112.10	105.0
112.90	174.0
114.70	127.0
115.70	627.0
116.70	1080.0
117.80	583.0
118.70	826.0
123.60	214.0
125.60	137.0
127.80	537.0
128.80	291.0
129.70	378.0
130.70	261.0
133.80	107.0
134.60	178.0
136.60	176.0
137.00	198.0
140.80	1406.0
142.80	2777.0
143.70	261.0
144.70	1391.0
145.70	362.0
147.80	213.0
148.80	104.0
149.80	127.0
151.70	106.0
152.70	212.0
153.70	168.0
154.80	284.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283

155.60	120.0
156.80	310.0
158.50	181.0
170.80	717.0
171.70	1793.0
172.90	2060.0
173.80	97920.0
174.90	6840.0
175.80	95048.0
176.80	6028.0

Instrument :
MSVOA_V
ClientSampleId :
BFB283