


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071818\
Data File : VV006627.D
Acq On : 18 Jul 2018 10:22
Operator : SY/MD
Sample : BFB67
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB67

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jul 19 02:39:44 2018

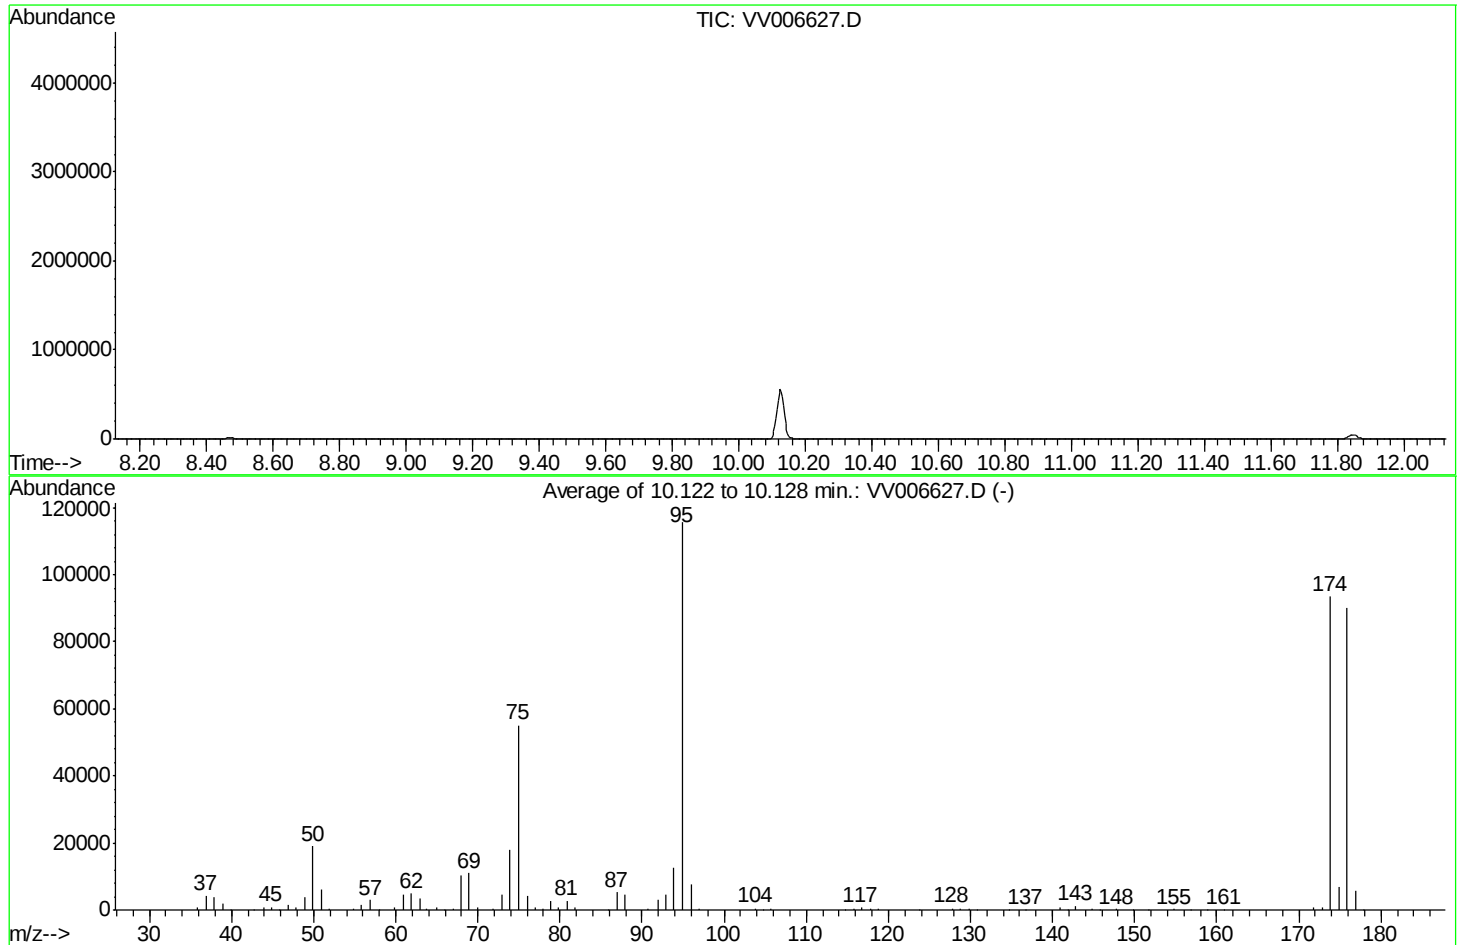

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	19016	PASS
75	95	30	80	47.7	55133	PASS
95	95	100	100	100.0	115632	PASS
96	95	5	9	6.7	7791	PASS
173	174	0.00	2	0.8	776	PASS
174	95	50	120	80.9	93520	PASS
175	174	5	9	7.2	6728	PASS
176	174	95	101	96.2	89989	PASS
177	176	5	9	6.4	5727	PASS

Scan 2858 (10.080 min): VV006627.D
BFB67

m/z	Abundance
39.80	210.0
40.90	111.0
41.80	118.0
43.90	575.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
35.90	806.0
36.90	4183.0
37.90	3799.0
38.90	1732.0
39.90	241.0
42.80	120.0
43.90	1173.0
44.80	802.0
45.90	126.0
46.90	1437.0
47.90	511.0
48.90	3809.0
49.90	18720.0
50.90	6185.0
51.90	349.0
54.90	314.0
55.80	1397.0
56.90	2814.0
57.90	133.0
59.80	976.0
60.90	4667.0
61.90	4720.0
62.90	3648.0
63.80	558.0
65.00	632.0
67.00	339.0
67.90	10065.0
68.90	10749.0
69.90	823.0
71.90	507.0
72.90	4701.0
73.90	17392.0
74.90	54072.0
76.00	4177.0
77.00	554.0
77.80	494.0
78.80	2559.0
79.80	862.0
80.90	2823.0
81.80	663.0
85.90	166.0
86.90	5078.0
87.80	4661.0
90.90	309.0
91.90	2891.0
92.90	4402.0
93.90	12503.0
94.90	111944.0
96.00	7691.0
97.00	220.0
103.80	357.0
104.70	131.0
105.70	314.0
115.80	298.0
116.70	612.0
117.80	364.0
118.70	472.0
127.70	414.0
128.80	191.0
129.80	336.0
130.80	112.0
134.70	192.0
136.70	159.0
140.90	820.0
141.90	104.0
142.80	1107.0
144.80	178.0
145.70	172.0
147.80	275.0
149.80	137.0
151.70	106.0
154.80	276.0
156.80	190.0
158.80	173.0
160.90	136.0
171.80	872.0
172.90	760.0
173.80	88200.0
174.90	6364.0
175.80	84688.0
176.90	5519.0
177.90	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
35.90	899.0
36.90	4538.0
37.90	4068.0
38.90	1845.0
39.80	210.0
42.70	105.0
43.90	1213.0
44.80	818.0
45.80	126.0
46.90	1621.0
47.90	619.0
48.90	4028.0
49.90	19720.0
50.90	6382.0
51.90	331.0
54.90	333.0
55.90	1417.0
56.90	3044.0
57.90	131.0
59.80	997.0
60.90	4726.0
61.90	4983.0
62.90	3740.0
63.80	519.0
65.00	693.0
65.90	103.0
67.00	296.0
67.90	10699.0
68.90	11448.0
69.90	927.0
71.90	556.0
72.90	4925.0
73.90	18528.0
74.90	57296.0
76.00	4454.0
77.00	615.0
77.90	525.0
78.80	2703.0
79.80	880.0
80.90	2904.0
81.80	737.0
86.00	176.0
86.90	5413.0
87.90	4852.0
90.70	305.0
91.90	3148.0
92.90	4640.0
93.90	13144.0
94.90	119816.0
95.90	8075.0
97.00	217.0
103.80	419.0
104.80	128.0
105.70	415.0
114.70	109.0
115.70	319.0
116.80	683.0
117.80	369.0
118.70	481.0
123.80	106.0
127.70	452.0
128.70	217.0
129.80	354.0
130.70	127.0
134.70	165.0
136.80	176.0
140.80	906.0
141.80	140.0
142.80	1231.0
144.80	218.0
145.80	157.0
147.80	277.0
149.80	130.0
154.80	307.0
156.80	208.0
158.80	202.0
160.90	137.0
171.90	940.0
172.90	787.0
173.90	96656.0
174.90	6964.0
175.80	93240.0
176.90	5916.0
177.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
35.90	862.0
36.90	4317.0
37.90	3944.0
38.90	1824.0
39.80	190.0
43.90	1172.0
44.90	832.0
45.80	127.0
46.90	1617.0
47.80	677.0
48.90	3812.0
49.90	18608.0
50.90	6003.0
51.90	290.0
54.90	297.0
55.90	1348.0
56.90	2830.0
57.90	113.0
59.90	914.0
60.90	4514.0
61.90	4796.0
62.90	3475.0
63.80	438.0
65.00	697.0
66.90	230.0
67.90	10172.0
68.90	10982.0
70.00	947.0
71.90	551.0
72.90	4676.0
73.90	17792.0
74.90	54032.0
76.00	4341.0
76.90	684.0
77.90	525.0
78.80	2574.0
79.80	806.0
80.80	2765.0
81.80	708.0
86.00	165.0
86.90	5290.0
87.90	4812.0
90.70	310.0
91.90	3066.0
92.90	4500.0
93.90	12524.0
94.90	115136.0
95.90	7608.0
96.90	207.0
103.90	460.0
104.80	124.0
105.70	482.0
114.70	109.0
115.70	328.0
116.80	690.0
117.80	358.0
118.80	447.0
127.80	446.0
128.70	205.0
129.80	340.0
130.70	135.0
134.70	135.0
136.80	189.0
140.80	894.0
141.80	146.0
142.80	1109.0
144.80	235.0
145.80	137.0
147.80	268.0
154.80	273.0
156.80	201.0
158.80	174.0
160.90	105.0
171.90	1011.0
172.90	781.0
173.90	95704.0
174.90	6858.0
175.80	92040.0
176.90	5746.0
177.80	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67