

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071819\
Quantitation Report (QT Reviewed)


Data File : VV011936.D
Acq On : 18 Jul 2019 16:16
Operator : SY/MD
Sample : K3823-13
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52N6

Manual Integrations
APPROVED

MMDadoda
7/22/2019 4:45:07 PM

Quant Time: Jul 19 06:41:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 19 05:34:55 2019
Response via : Initial Calibration

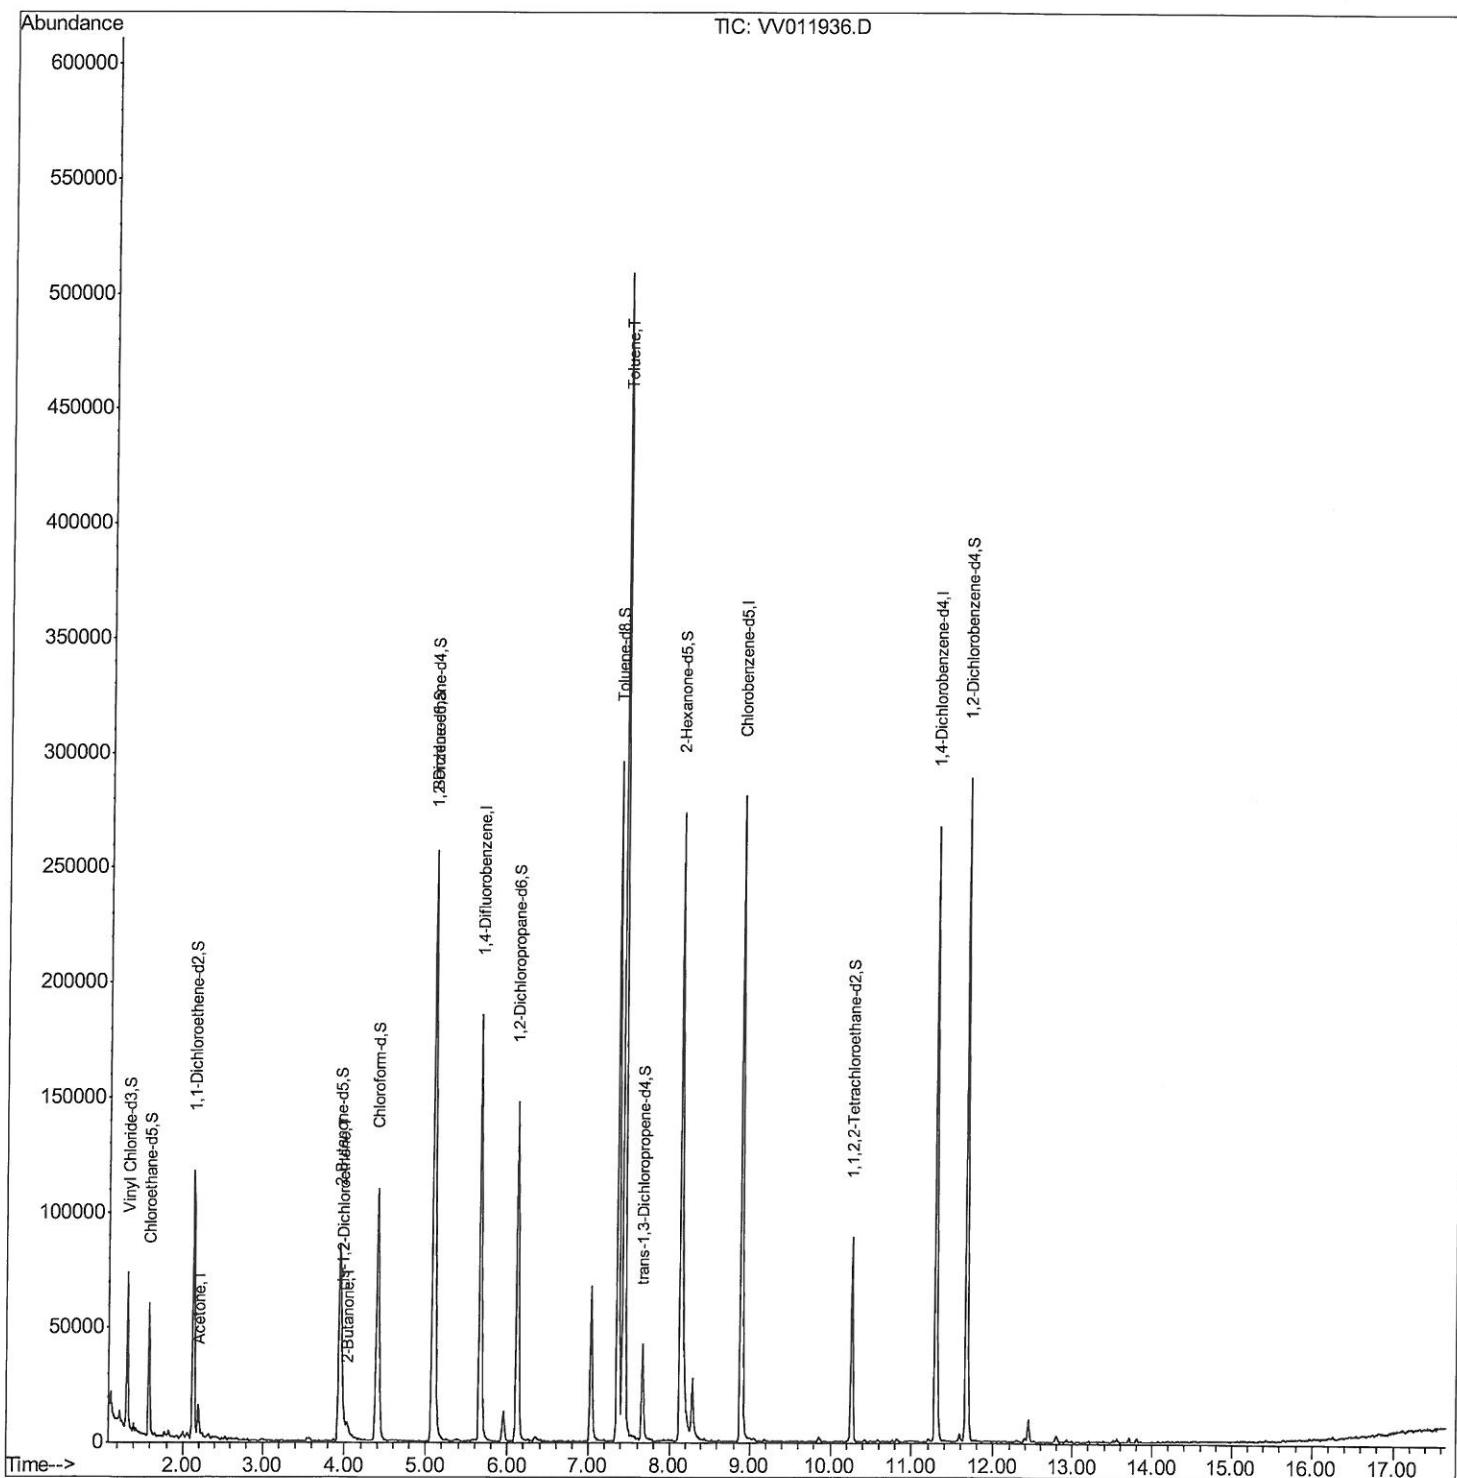

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071819\
Quantitation Report (Qedit)




Data File : VV011936.D
Acq On : 18 Jul 2019 16:16
Operator : SY/MD
Sample : K3823-13
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
A52N6

Manual Integrations
APPROVED

MMDadoda
7/22/2019 4:45:07 PM

Quant Time: Jul 19 05:47:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 19 05:34:55 2019
Response via : Initial Calibration

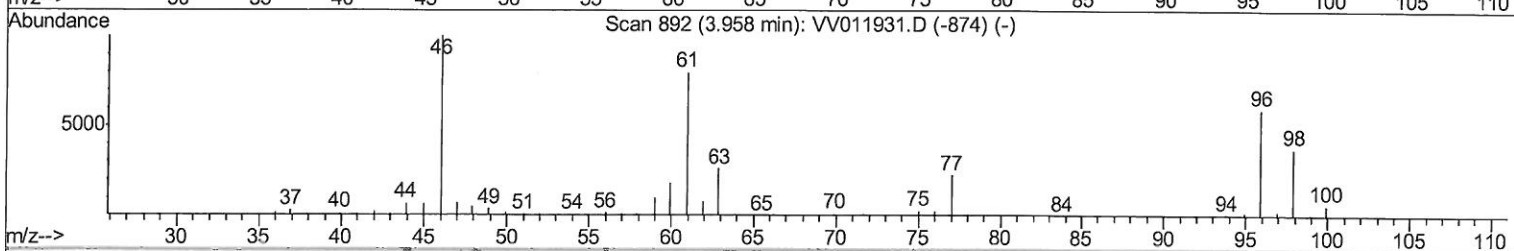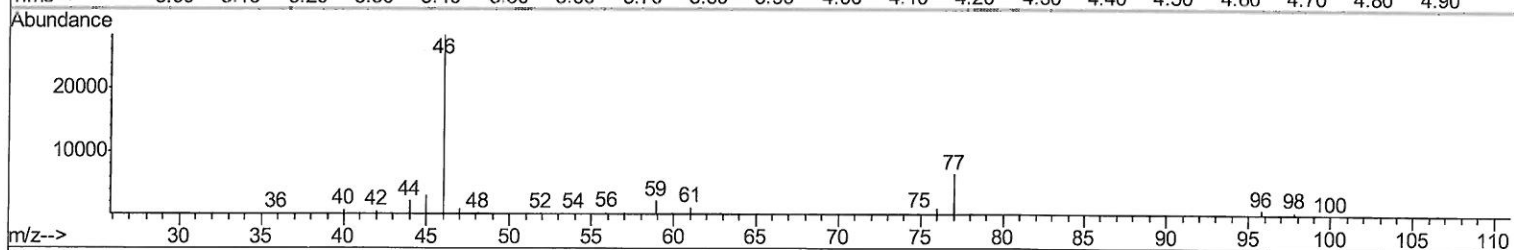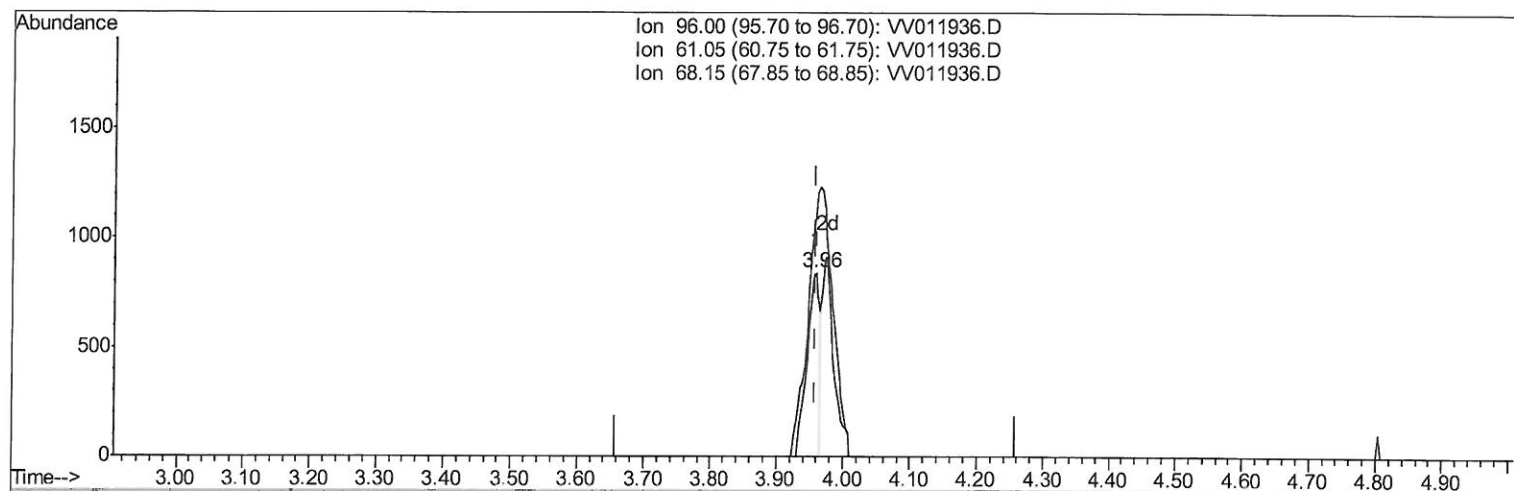

TIC: VV011936.D

(22) cis-1,2-Dichloroethene (T)

3.958min (+0.000) 0.09ug/L

response 1094

Ion	Exp%	Act%
96.00	100	100
61.05	136.00	133.73
68.15	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071819\
Quantitation Report (Qedit)




Data File : VV011936.D
Acq On : 18 Jul 2019 16:16
Operator : SY/MD
Sample : K3823-13
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52N6

Manual Integrations
APPROVED

MMDadoda
7/22/2019 4:45:07 PM

Quant Time: Jul 19 05:47:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 19 05:34:55 2019
Response via : Initial Calibration

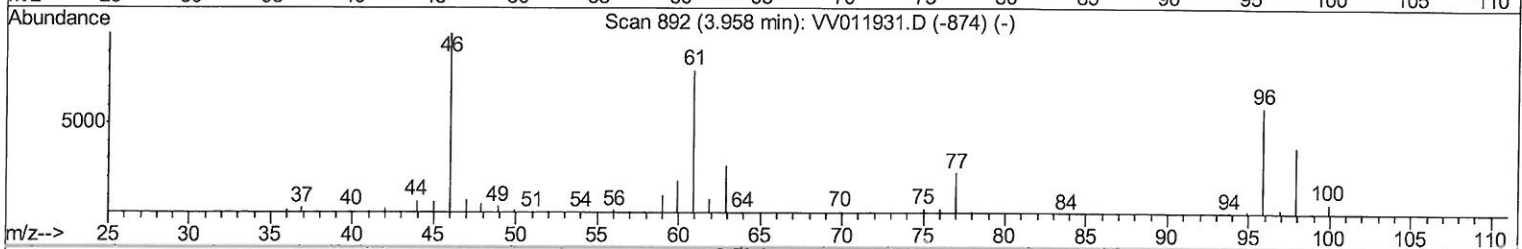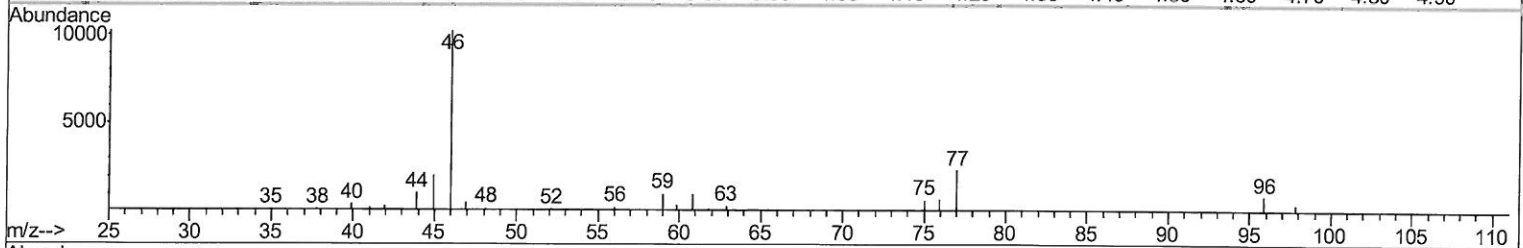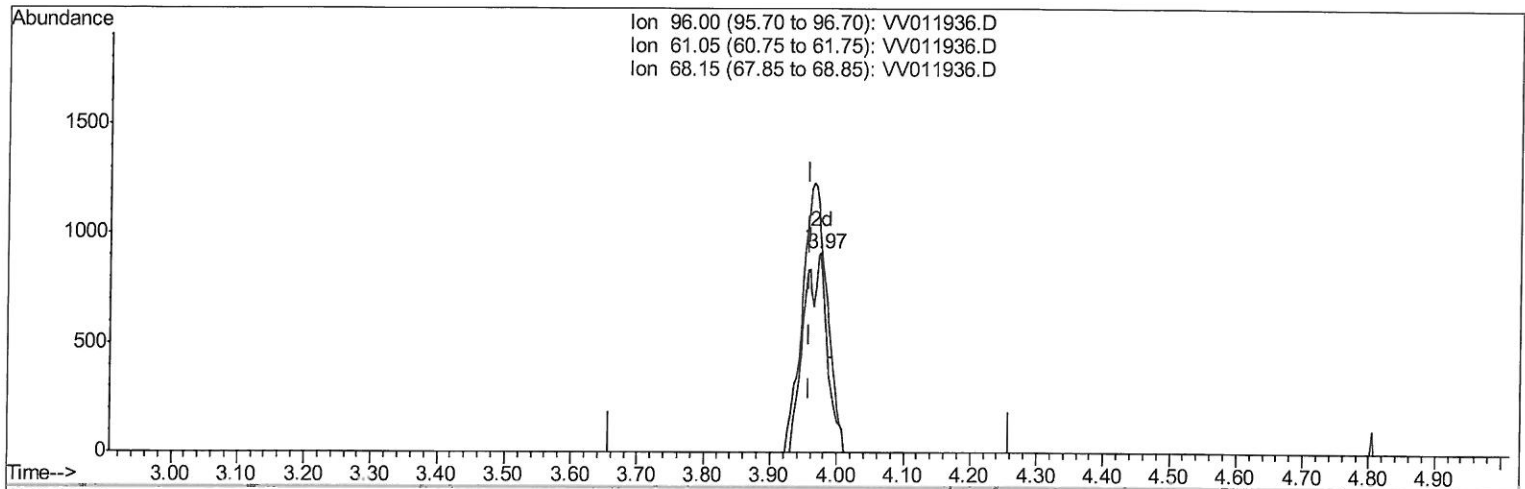

TIC: VV011936.D

(22) cis-1,2-Dichloroethene (T)

3.974min (+0.016) 0.19ug/L m

response 2221

Ion Exp% Act%

96.00 100 100

61.05 136.00 109.98

68.15 0.00 0.00

0.00 0.00 0.00

Handwritten: 7 MD / 7/23/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV071819\

Quantitation Report (QT Reviewed)

Data File : VV011936.D

Acq On : 18 Jul 2019 16:16

Operator : SY/MD

Sample : K3823-13

Misc : 25ML/MSVOA_V/WATER

ALS Vial : 7 Sample Multiplier: 1

Instrument :

MSVOA_V

ClientSampleId :

A52N6

Manual Integrations

APPROVED

MMDadoda

7/22/2019 4:45:07 PM

Quant Time: Jul 19 06:41:37 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Fri Jul 19 05:34:55 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	155348	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	148870	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	69489	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	41635	3.65	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	73.00%
7) Chloroethane-d5	1.59	69	33732	3.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	71.40%
11) 1,1-Dichloroethene-d2	2.13	63	61317	3.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.60%
20) 2-Butanone-d5	3.94	46	137251	47.63	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.26%
24) Chloroform-d	4.40	84	109637	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.08	65	58655	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.00%
32) Benzene-d6	5.10	84	221183	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	6.12	67	67056	5.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.00%
41) Toluene-d8	7.36	98	191188	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
43) trans-1,3-Dichloropropene-	7.67	79	23191	4.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.40%
46) 2-Hexanone-d5	8.14	63	95656	48.39	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.78%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	39012	4.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	75417	5.43	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.60%

Target Compounds

					Qvalue
13) Acetone	2.19	43	12297	8.409	ug/L 97
21) 2-Butanone	4.04	43	8690	3.031	ug/L 95
22) cis-1,2-Dichloroethene	3.97	96	2221m	0.185	ug/L 100
42) Toluene	7.43	91	356035	7.284	ug/L

2 MD
7/23/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed