

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071819\
 Data File : VV011933.D
 Acq On : 18 Jul 2019 14:58
 Operator : SY/MD
 Sample : K3772-02
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jul 19 05:57:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 19 05:34:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	158637	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	151202	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	65983	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	56314	4.83	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	96.60%
7) Chloroethane-d5	1.58	69	50000	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.60%
11) 1,1-Dichloroethene-d2	2.13	63	70677	3.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.20%
20) 2-Butanone-d5	3.96	46	173733	59.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.08%
24) Chloroform-d	4.40	84	122329	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
26) 1,2-Dichloroethane-d4	5.08	65	68747	5.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.80%
32) Benzene-d6	5.09	84	246330	5.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.00%
36) 1,2-Dichloropropane-d6	6.12	67	76525	5.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.60%
41) Toluene-d8	7.36	98	206972	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.00%
43) trans-1,3-Dichloropropene-	7.66	79	25942	5.20	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	104.00%
46) 2-Hexanone-d5	8.13	63	110001	54.79	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.58%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	43868	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	74502	5.65	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.00%


Target Compounds					Ovalue
16) Methylene chloride	2.53	84	3128	0.353 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071819\
Data File : VV011933.D
Acq On : 18 Jul 2019 14:58
Operator : SY/MD
Sample : K3772-02
Misc : 25ML/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jul 19 05:57:29 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 19 05:34:55 2019
Response via : Initial Calibration

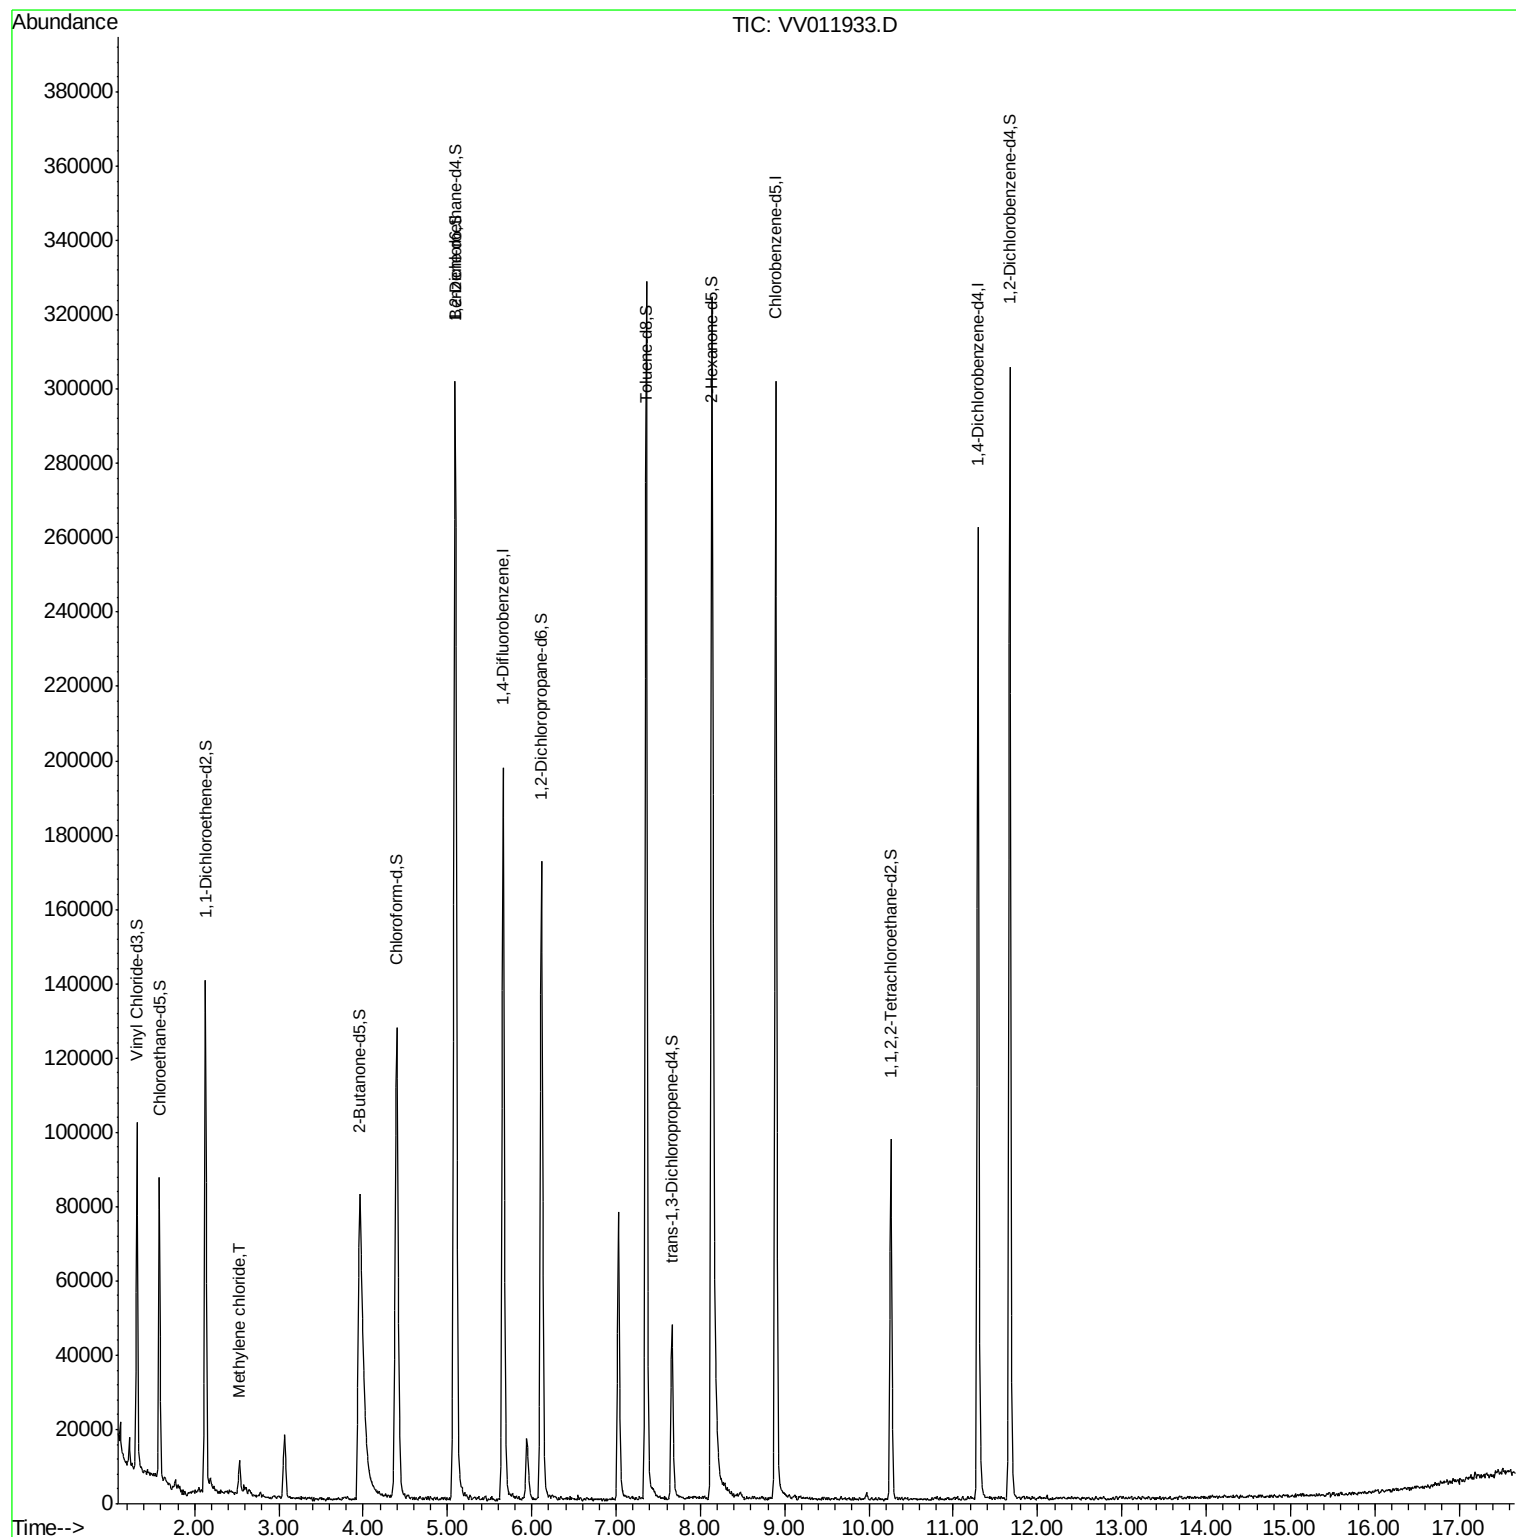

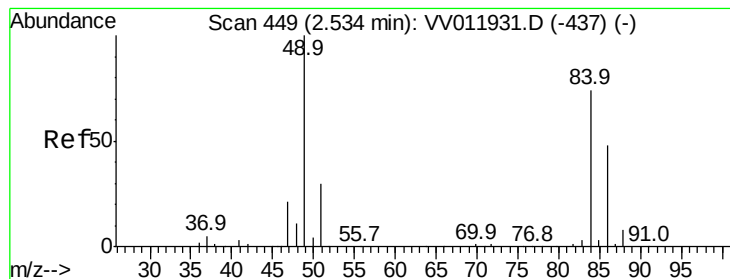

#16
 Methvlene chloride
 Concen: 0.353 ug/L
 RT: 2.53 min Scan# 448
 Delta R.T. -0.00 min
 Lab File: VV011933.D
 Acq: 18 Jul 2019 14:58

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 84 Resp: 3128
 Ion Ratio Lower Upper
 84 100
 86 58.7 44.8 83.2
 49 117.9 90.4 168.0

