

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071819\
 Data File : VV011941.D
 Acq On : 18 Jul 2019 18:18
 Operator : SY/MD
 Sample : K3823-11DL 50X
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A52L8DL

Quant Time: Jul 19 06:57:55 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 19 05:34:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	131266	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	123609	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	57714	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	31790	3.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.00%
7) Chloroethane-d5	1.58	69	26528	3.32	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	66.40%
11) 1,1-Dichloroethene-d2	2.13	63	51247	3.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.00%
20) 2-Butanone-d5	3.95	46	125857	51.69	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.38%
24) Chloroform-d	4.40	84	98752	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.20%
26) 1,2-Dichloroethane-d4	5.08	65	54171	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.20%
32) Benzene-d6	5.10	84	191286	5.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.40%
36) 1,2-Dichloropropane-d6	6.12	67	57517	5.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.40%
41) Toluene-d8	7.36	98	164355	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
43) trans-1,3-Dichloropropene-	7.67	79	19244	4.72	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.40%
46) 2-Hexanone-d5	8.14	63	81616	49.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.44%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35714	5.16	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	68452	5.94	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.80%


Target Compounds					Ovalue
22) cis-1,2-Dichloroethene	3.96	96	98303	9.707 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071819\
Data File : VV011941.D
Acq On : 18 Jul 2019 18:18
Operator : SY/MD
Sample : K3823-11DL 50X
Misc : 25ML/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52L8DL

Quant Time: Jul 19 06:57:55 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 19 05:34:55 2019
Response via : Initial Calibration

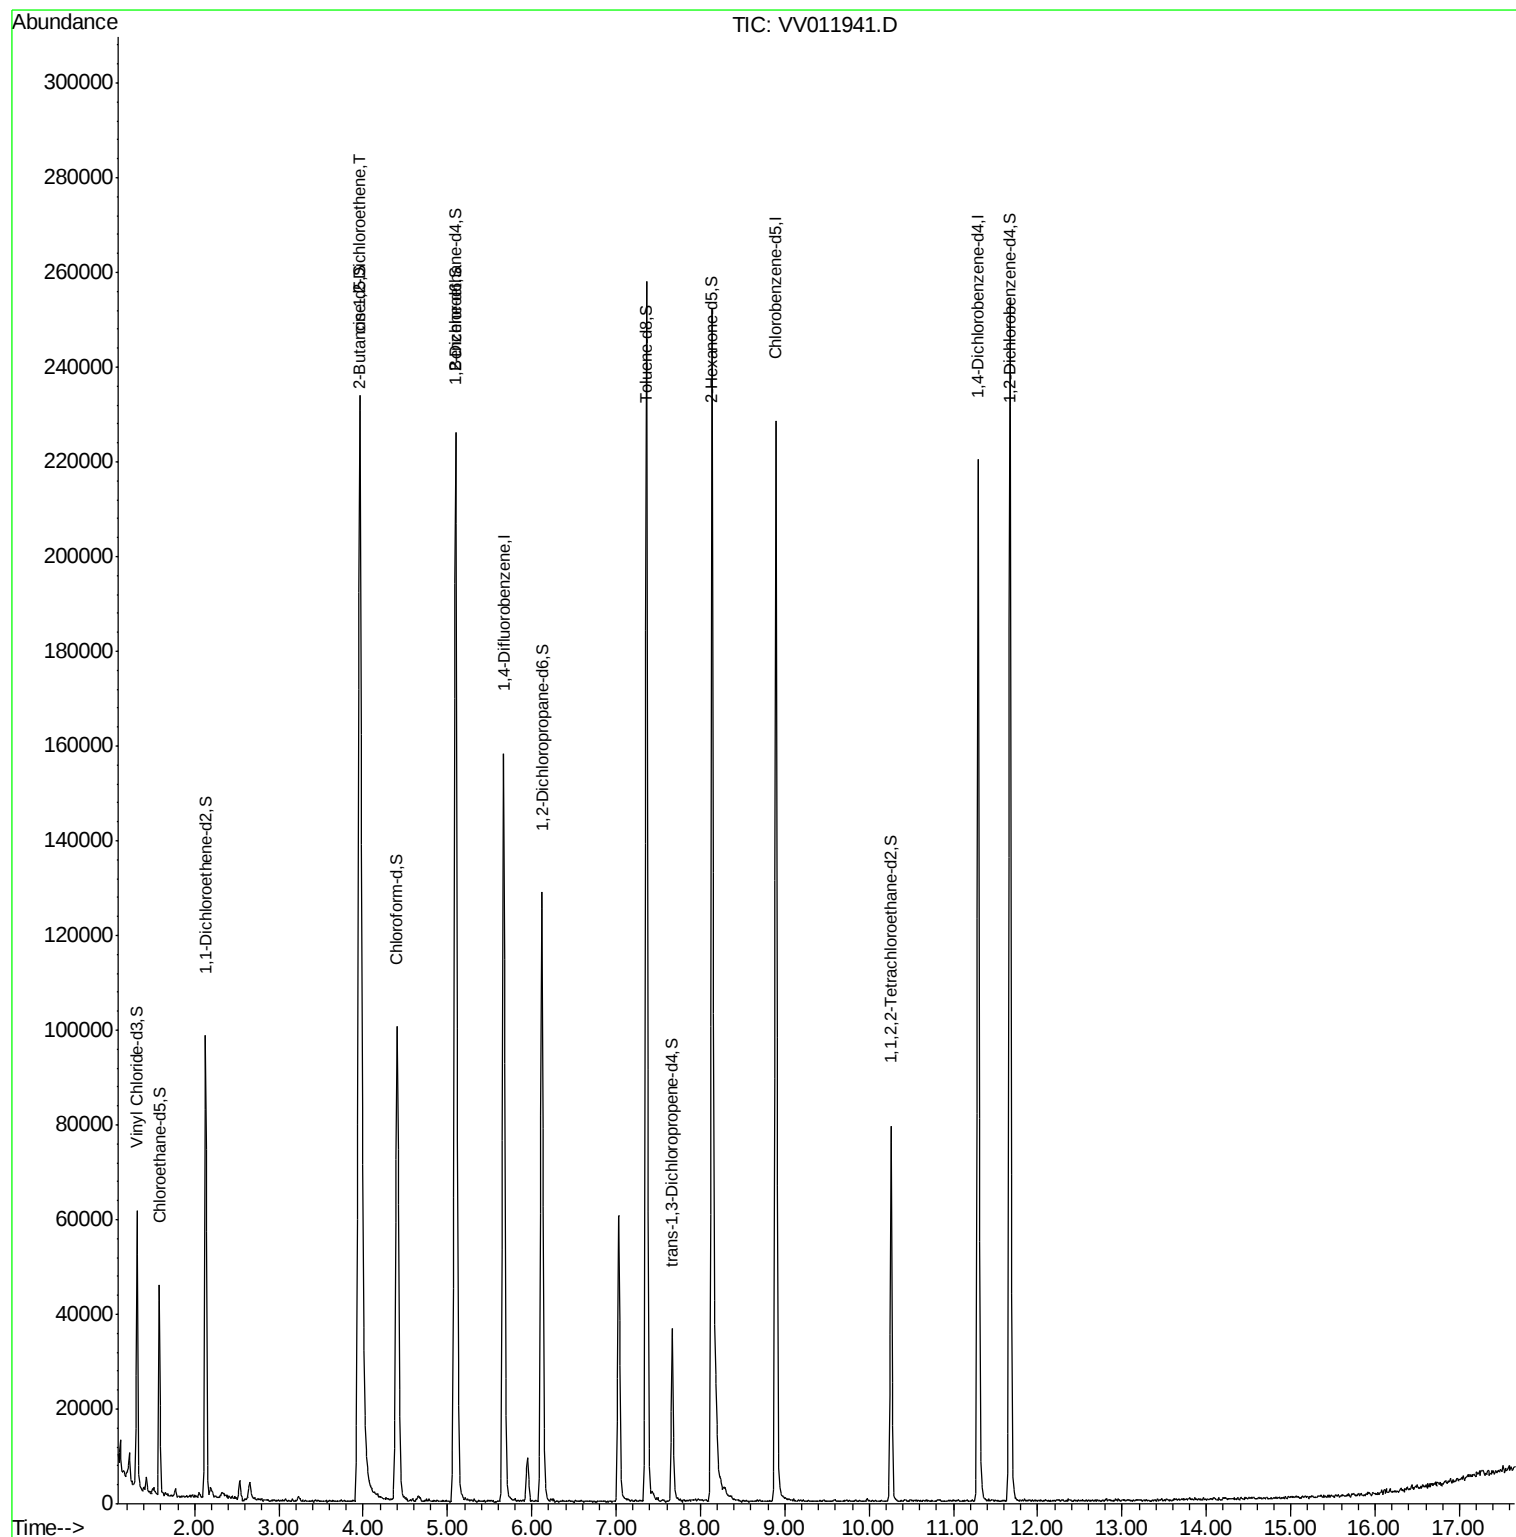

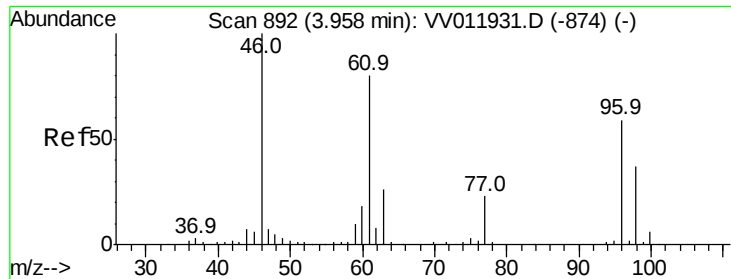

#22

cis-1,2-Dichloroethene
 Concen: 9.707 ug/L
 RT: 3.96 min Scan# 894
 Delta R.T. 0.01 min
 Lab File: VV011941.D
 Acq: 18 Jul 2019 18:18

Instrument :
 MSVOA_V
 ClientSampleId :
 A52L8DL

Tot Ion: 96 Resp: 98303
 Ion Ratio Lower Upper
 96 100
 61 131.4 95.2 176.8
 68 0.0 0.0 0.0

