

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071819\
 Data File : VV011944.D
 Acq On : 18 Jul 2019 19:32
 Operator : SY/MD
 Sample : K3823-08DL 200X
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A52K8DL

Quant Time: Jul 19 07:09:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jul 19 05:34:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	105263	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	101444	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	47259	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	30864	3.99	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.80%
7) Chloroethane-d5	1.58	69	26302	4.11	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.20%
11) 1,1-Dichloroethene-d2	2.13	63	51139	4.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.80%
20) 2-Butanone-d5	3.96	46	128461	65.79	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	131.58%#
24) Chloroform-d	4.40	84	97147	6.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	125.40%#
26) 1,2-Dichloroethane-d4	5.08	65	54583	6.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	137.20%#
32) Benzene-d6	5.10	84	189660	6.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	128.40%#
36) 1,2-Dichloropropane-d6	6.12	67	58267	6.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	128.80%
41) Toluene-d8	7.36	98	163442	6.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	121.40%
43) trans-1,3-Dichloropropene-	7.67	79	20376	6.09	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	121.80%
46) 2-Hexanone-d5	8.14	63	83076	61.67	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	123.34%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35680	6.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	125.60%#
64) 1,2-Dichlorobenzene-d4	11.67	152	65602	6.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	139.00%#


Target Compounds					Ovalue
22) cis-1,2-Dichloroethene	3.96	96	87297	10.750 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV071819\
Data File : VV011944.D
Acq On : 18 Jul 2019 19:32
Operator : SY/MD
Sample : K3823-08DL 200X
Misc : 25ML/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A52K8DL

Quant Time: Jul 19 07:09:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jul 19 05:34:55 2019
Response via : Initial Calibration

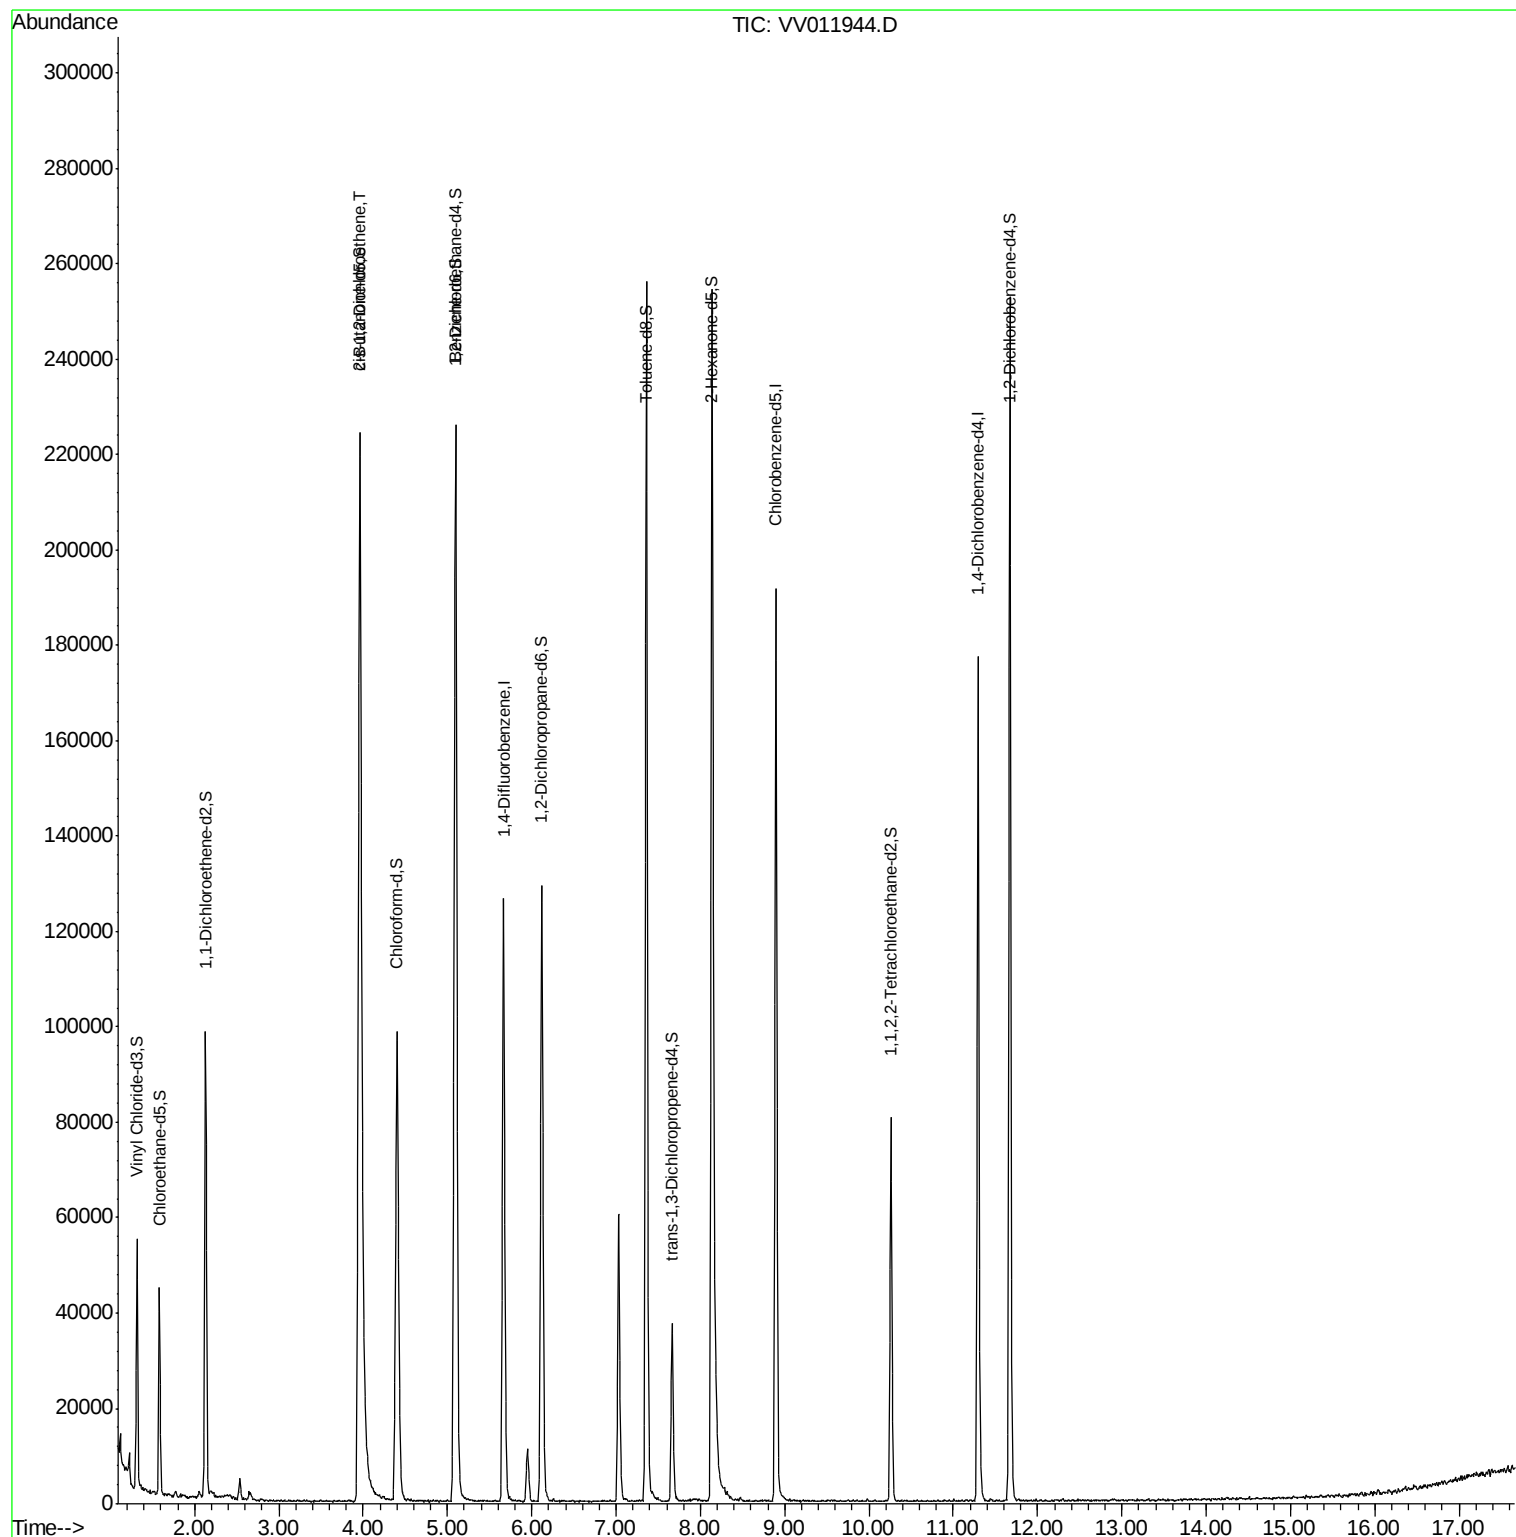

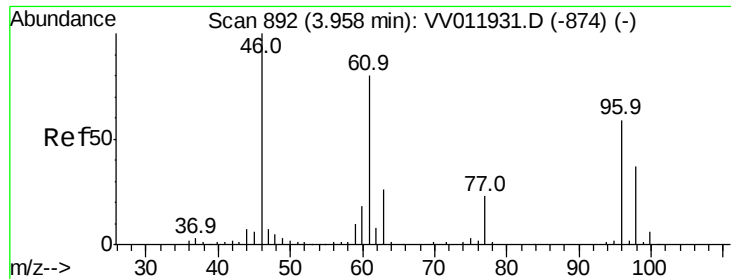

#22
 cis-1,2-Dichloroethene
 Concen: 10.750 ug/L
 RT: 3.96 min Scan# 893
 Delta R.T. 0.00 min
 Lab File: VV011944.D
 Acq: 18 Jul 2019 19:32

Instrument :
 MSVOA_V
 ClientSampleId :
 A52K8DL

Tot Ion: 96 Resp: 87297
 Ion Ratio Lower Upper
 96 100
 61 129.7 95.2 176.8
 68 0.0 0.0 0.0

