


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV071819\
 Data File : VV011930.D
 Acq On : 18 Jul 2019 10:01
 Operator : SY/MD
 Sample : BFB35
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB35

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071719WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jul 19 05:34:55 2019

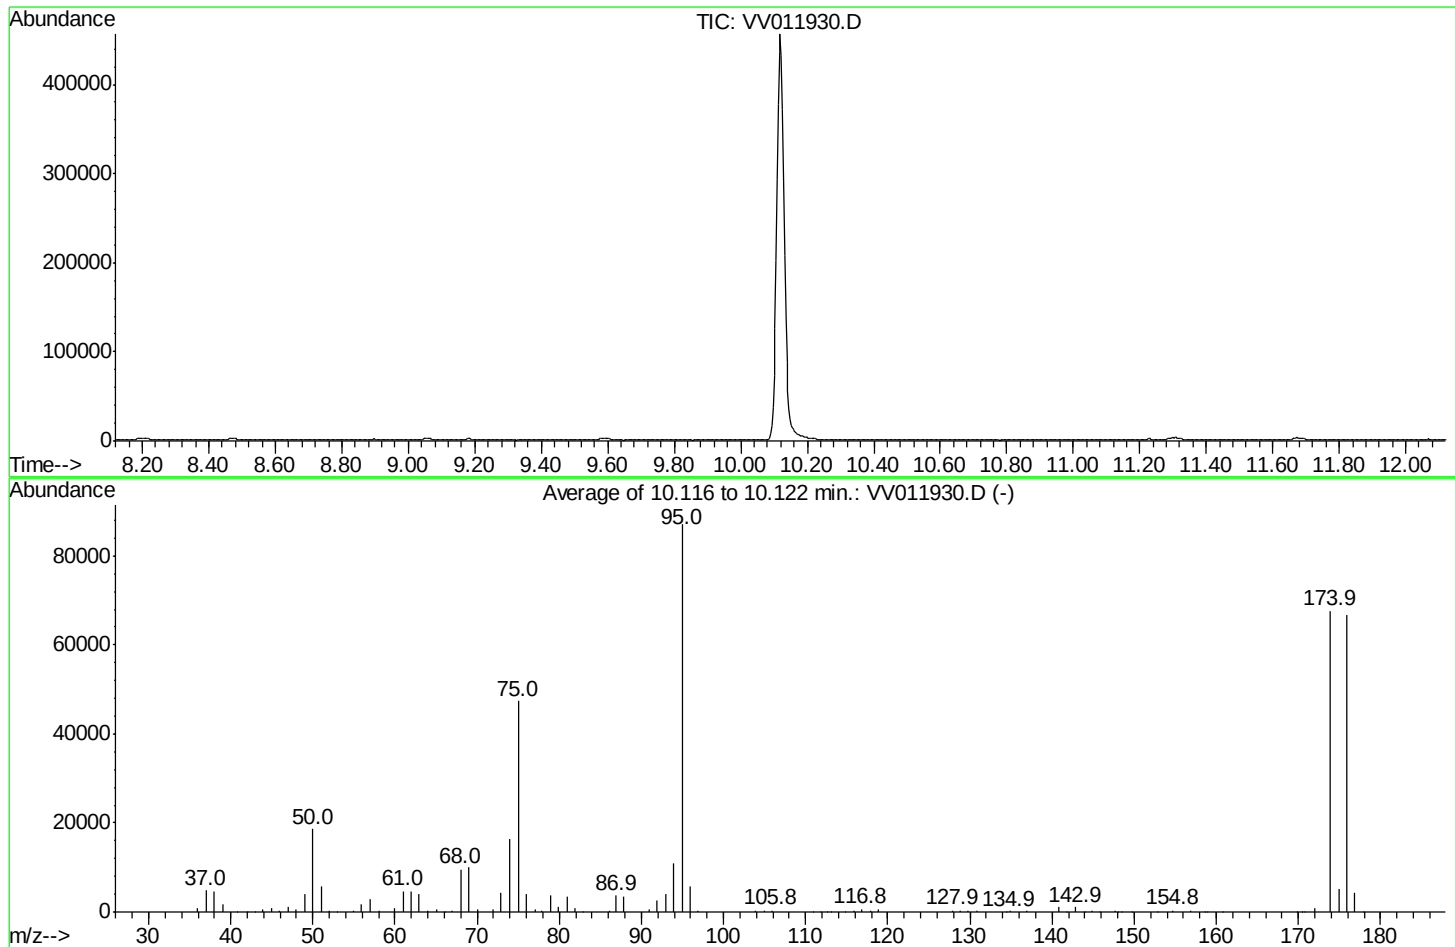

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	18613	PASS
75	95	30	80	54.4	47416	PASS
95	95	100	100	100.0	87085	PASS
96	95	5	9	6.5	5703	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.8	67722	PASS
175	174	5	9	7.4	5044	PASS
176	174	95	101	98.5	66682	PASS
177	176	5	9	6.7	4455	PASS

Scan 2794 (10.074 min): VV011930.D
BFB35

m/z	Abundance
36.20	141.0
39.00	123.0
39.80	473.0
43.90	428.0
52.70	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
36.00	969.0
37.00	4928.0
38.00	4848.0
39.00	1923.0
40.00	497.0
40.80	113.0
42.00	128.0
43.00	135.0
43.90	1111.0
45.00	834.0
45.90	203.0
47.00	1245.0
47.80	651.0
48.90	4262.0
50.00	18608.0
51.00	5639.0
52.00	406.0
53.00	159.0
54.90	342.0
56.00	1633.0
57.00	2882.0
58.10	225.0
59.90	812.0
61.00	4643.0
62.00	4509.0
63.00	3865.0
63.90	496.0
65.00	732.0
66.10	125.0
66.90	317.0
68.00	9174.0
69.00	9810.0
70.00	738.0
72.00	684.0
72.90	4550.0
74.00	16358.0
75.00	47224.0
76.00	3912.0
77.00	500.0
77.90	319.0
78.90	3624.0
79.90	1025.0
80.90	3611.0
81.90	864.0
82.80	145.0
86.10	171.0
86.90	3617.0
87.90	3408.0
90.90	453.0
91.90	2794.0
92.90	4012.0
94.00	11150.0
95.00	87128.0
96.00	5798.0
96.90	162.0
103.90	360.0
104.90	209.0
105.90	437.0
110.80	127.0
112.70	116.0
113.00	110.0
114.90	148.0
115.80	334.0
116.80	679.0
117.90	431.0
118.80	517.0
127.90	399.0
128.70	183.0
129.80	352.0
130.90	203.0
134.50	141.0
134.90	166.0
137.00	278.0
140.80	974.0
141.70	143.0
142.90	1022.0
143.90	114.0
144.80	255.0
145.80	130.0
147.70	135.0
148.00	127.0
149.70	109.0
154.70	272.0
156.80	228.0
158.60	108.0
160.80	130.0
169.80	114.0
170.80	140.0
171.90	791.0
173.90	65032.0
174.90	5007.0
175.90	64088.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

176.90

177.90

4349.0

174.0

Instrument :

MSVOA_V

ClientSampleId :

BFB35

m/z	Abundance
36.00	952.0
37.00	5026.0
38.00	4817.0
39.00	1962.0
40.00	455.0
40.80	136.0
41.90	107.0
43.00	136.0
43.90	1020.0
45.00	931.0
45.80	198.0
47.00	1320.0
47.90	579.0
48.90	4266.0
50.00	19312.0
51.00	5823.0
52.00	365.0
52.90	150.0
54.90	306.0
55.90	1740.0
56.90	2909.0
58.00	192.0
59.90	806.0
61.00	4846.0
62.00	4735.0
62.90	4140.0
64.00	422.0
65.00	687.0
66.00	137.0
66.90	318.0
68.00	9868.0
69.00	10241.0
70.00	716.0
72.00	709.0
72.90	4556.0
74.00	16896.0
75.00	49056.0
76.00	4142.0
77.00	510.0
77.90	403.0
78.90	3751.0
79.90	1070.0
80.90	3675.0
81.90	804.0
82.80	122.0
86.00	208.0
86.90	3811.0
87.90	3584.0
90.90	459.0
91.90	2760.0
92.90	4151.0
94.00	11477.0
95.00	89888.0
96.00	5900.0
96.90	195.0
103.90	391.0
105.00	228.0
105.80	441.0
110.80	137.0
111.80	133.0
112.60	125.0
114.90	140.0
115.90	388.0
116.80	730.0
117.90	402.0
118.80	527.0
127.90	387.0
128.80	208.0
129.70	332.0
130.90	178.0
134.90	181.0
136.90	261.0
140.80	1060.0
141.80	133.0
142.90	1057.0
144.80	292.0
145.80	140.0
147.70	169.0
152.90	104.0
154.80	345.0
156.80	261.0
158.90	106.0
160.80	127.0
169.90	103.0
170.50	130.0
171.90	852.0
173.90	69992.0
174.90	5231.0
175.90	68968.0
176.90	4571.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35

m/z	Abundance
35.90	859.0
37.00	4713.0
38.00	4286.0
39.00	1868.0
40.00	410.0
40.80	127.0
41.90	121.0
43.00	153.0
43.90	904.0
45.00	936.0
45.80	147.0
47.00	1256.0
48.00	483.0
49.00	3840.0
50.00	17920.0
51.00	5455.0
52.00	313.0
53.00	143.0
54.90	251.0
55.90	1653.0
56.90	2638.0
57.90	209.0
60.00	832.0
60.90	4532.0
61.90	4517.0
62.90	3852.0
64.00	375.0
65.00	627.0
66.00	138.0
67.00	300.0
68.00	9460.0
69.00	9934.0
70.00	600.0
72.00	665.0
72.90	4040.0
74.00	15550.0
75.00	45968.0
76.00	3940.0
77.10	463.0
77.90	429.0
78.90	3477.0
79.90	1030.0
80.90	3373.0
81.90	680.0
82.90	116.0
86.00	197.0
86.90	3663.0
87.90	3471.0
90.90	441.0
91.90	2539.0
92.90	4184.0
93.90	10523.0
95.00	84240.0
96.00	5412.0
96.90	229.0
103.80	383.0
105.00	206.0
105.80	440.0
110.90	141.0
111.90	136.0
112.60	122.0
114.70	118.0
115.90	423.0
116.80	720.0
117.90	394.0
118.80	517.0
127.90	330.0
128.80	200.0
129.80	281.0
130.80	152.0
134.90	172.0
136.80	260.0
140.80	1023.0
142.90	1009.0
144.90	280.0
145.80	132.0
147.80	217.0
148.50	104.0
152.90	127.0
154.80	350.0
156.90	235.0
158.90	108.0
160.80	108.0
170.40	144.0
172.00	783.0
173.90	68144.0
174.90	4894.0
175.90	66992.0
176.90	4447.0
177.90	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB35