

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
 Data File : VV026813.D
 Acq On : 18 Jul 2022 16:03
 Operator : SY/MD
 Sample : VIBLK276
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK276

Quant Time: Jul 19 03:11:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jul 19 03:06:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	259656	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	257259	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	105654	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	89313	3.770	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.400%
7) Chloroethane-d5	1.564	69	84244	4.116	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.400%
11) 1,1-Dichloroethene-d2	2.101	63	120559	2.651	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.000%#
20) 2-Butanone-d5	3.889	46	193158	52.246	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.500%
24) Chloroform-d	4.346	84	182955	4.417	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
26) 1,2-Dichloroethane-d4	5.030	65	84836	4.688	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%
32) Benzene-d6	5.047	84	334028	4.273	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.400%
36) 1,2-Dichloropropane-d6	6.069	67	111115	4.741	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.800%
41) Toluene-d8	7.317	98	247751	3.570	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.400%
43) trans-1,3-Dichloroprop...	7.625	79	31180	4.066	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.400%
46) 2-Hexanone-d5	8.088	63	152103	45.813	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.620%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	84345	4.619	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	92226	5.010	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.200%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	23055	0.850	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026813.D
Acq On : 18 Jul 2022 16:03
Operator : SY/MD
Sample : VIBLK276
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Time: Jul 19 03:11:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 19 03:06:10 2022
Response via : Initial Calibration

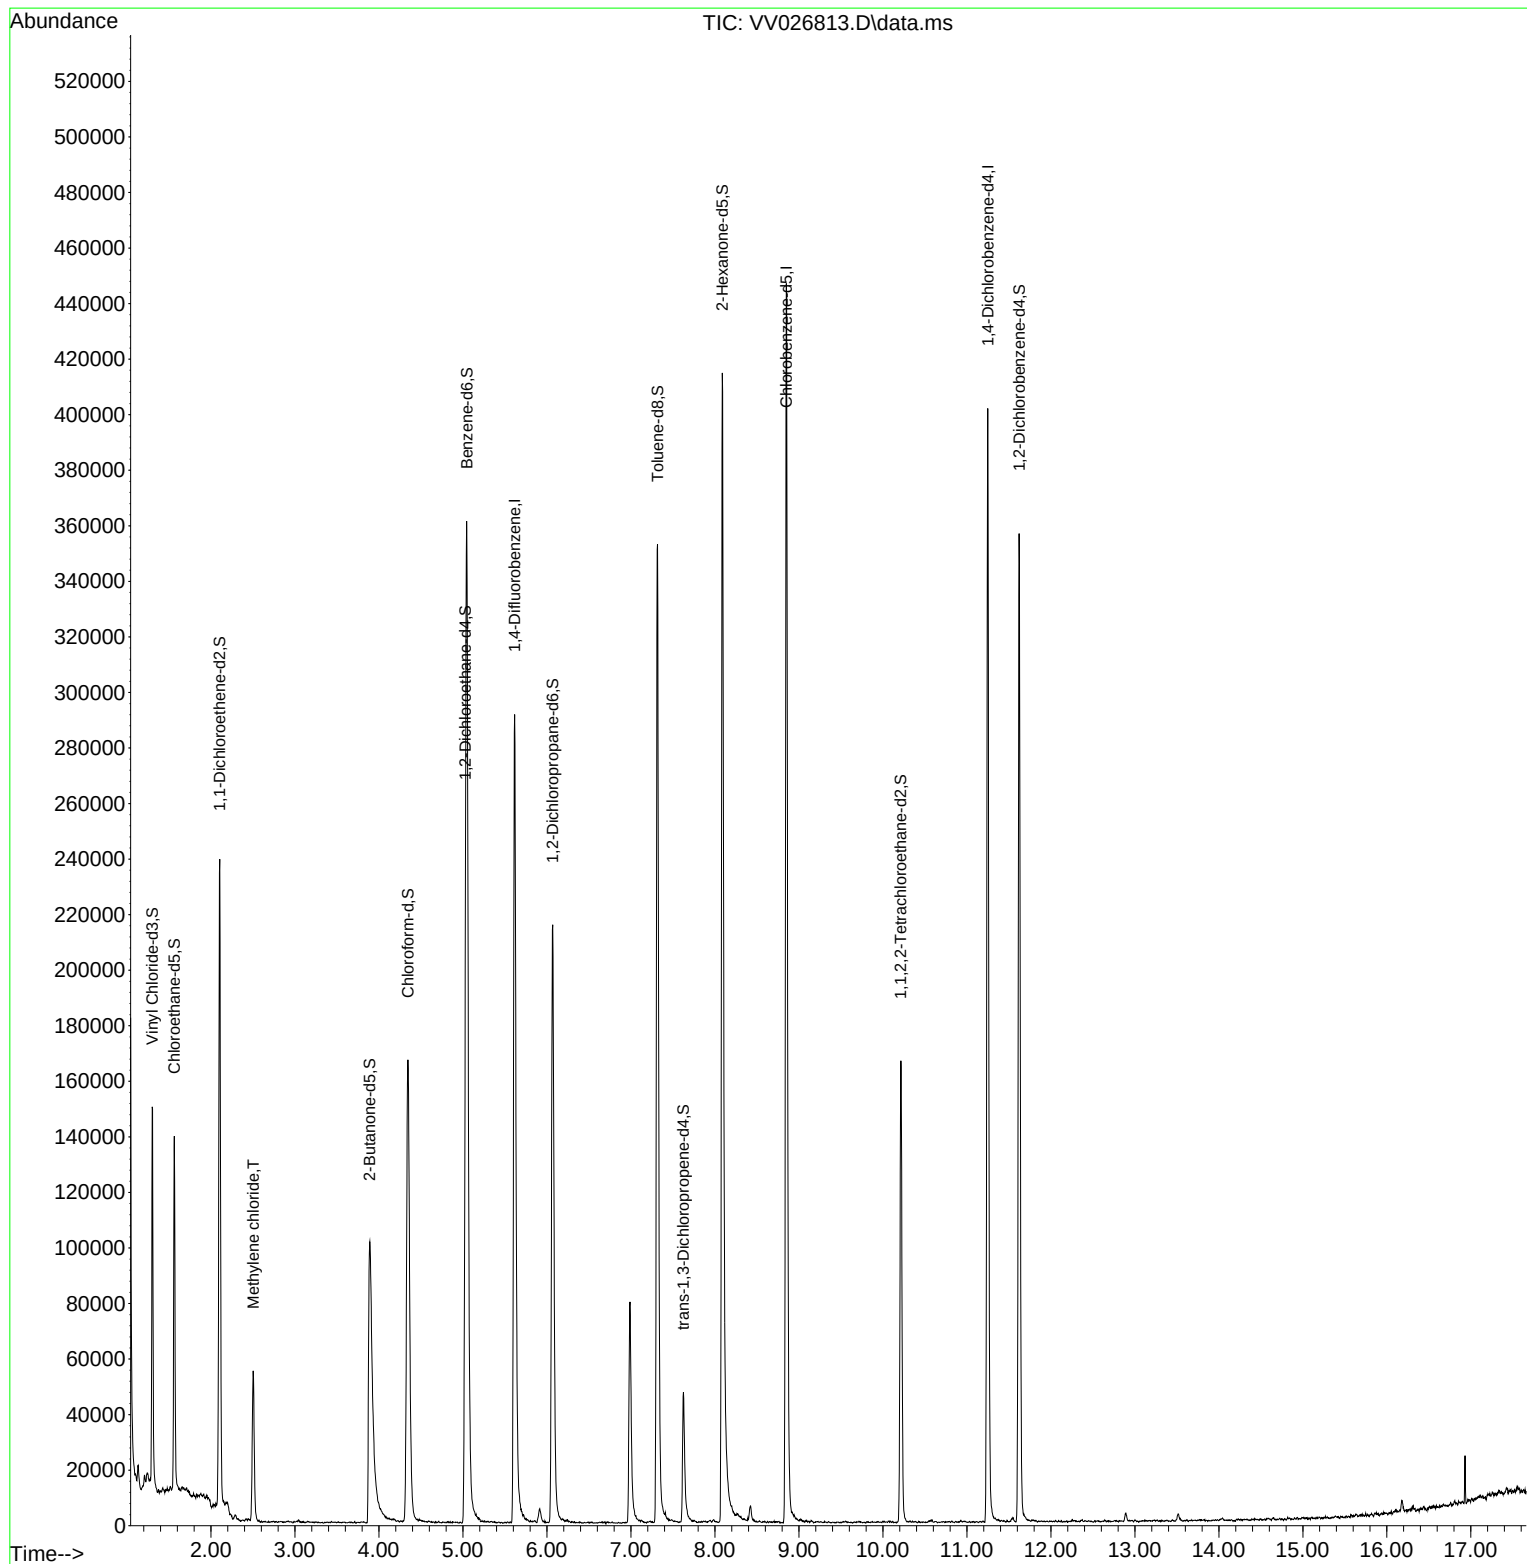

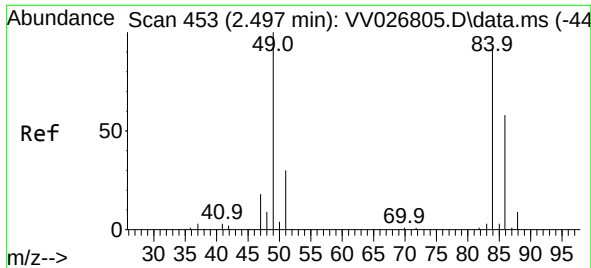

#16
Methylene chloride
Concen: 0.850 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV026813.D
Acq: 18 Jul 2022 16:03

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Tgt Ion: 84 Resp: 23055
Ion Ratio Lower Upper
84 100
86 63.1 44.8 83.2
49 117.4 78.7 146.1

