

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071822\
 Data File : VW026814.D
 Acq On : 18 Jul 2022 16:32
 Operator : SY/MD
 Sample : N3739-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jul 19 04:46:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jul 19 03:06:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	280661	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	268357	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	107031	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	111210	4.343	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.800%
7) Chloroethane-d5	1.564	69	103683	4.687	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.800%
11) 1,1-Dichloroethene-d2	2.101	63	148304	3.017	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.400%
20) 2-Butanone-d5	3.896	46	181380	45.389	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.780%
24) Chloroform-d	4.343	84	221699	4.952	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
26) 1,2-Dichloroethane-d4	5.027	65	90773	4.641	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
32) Benzene-d6	5.043	84	402199	4.932	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.600%
36) 1,2-Dichloropropane-d6	6.066	67	127688	5.223	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.400%
41) Toluene-d8	7.313	98	297166	4.105	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	7.625	79	32591	4.074	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.400%
46) 2-Hexanone-d5	8.088	63	137559	39.719	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.440%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	80774	4.241	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	108782	5.833	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.600%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	7059	0.241	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026814.D
Acq On : 18 Jul 2022 16:32
Operator : SY/MD
Sample : N3739-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jul 19 04:46:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 19 03:06:10 2022
Response via : Initial Calibration

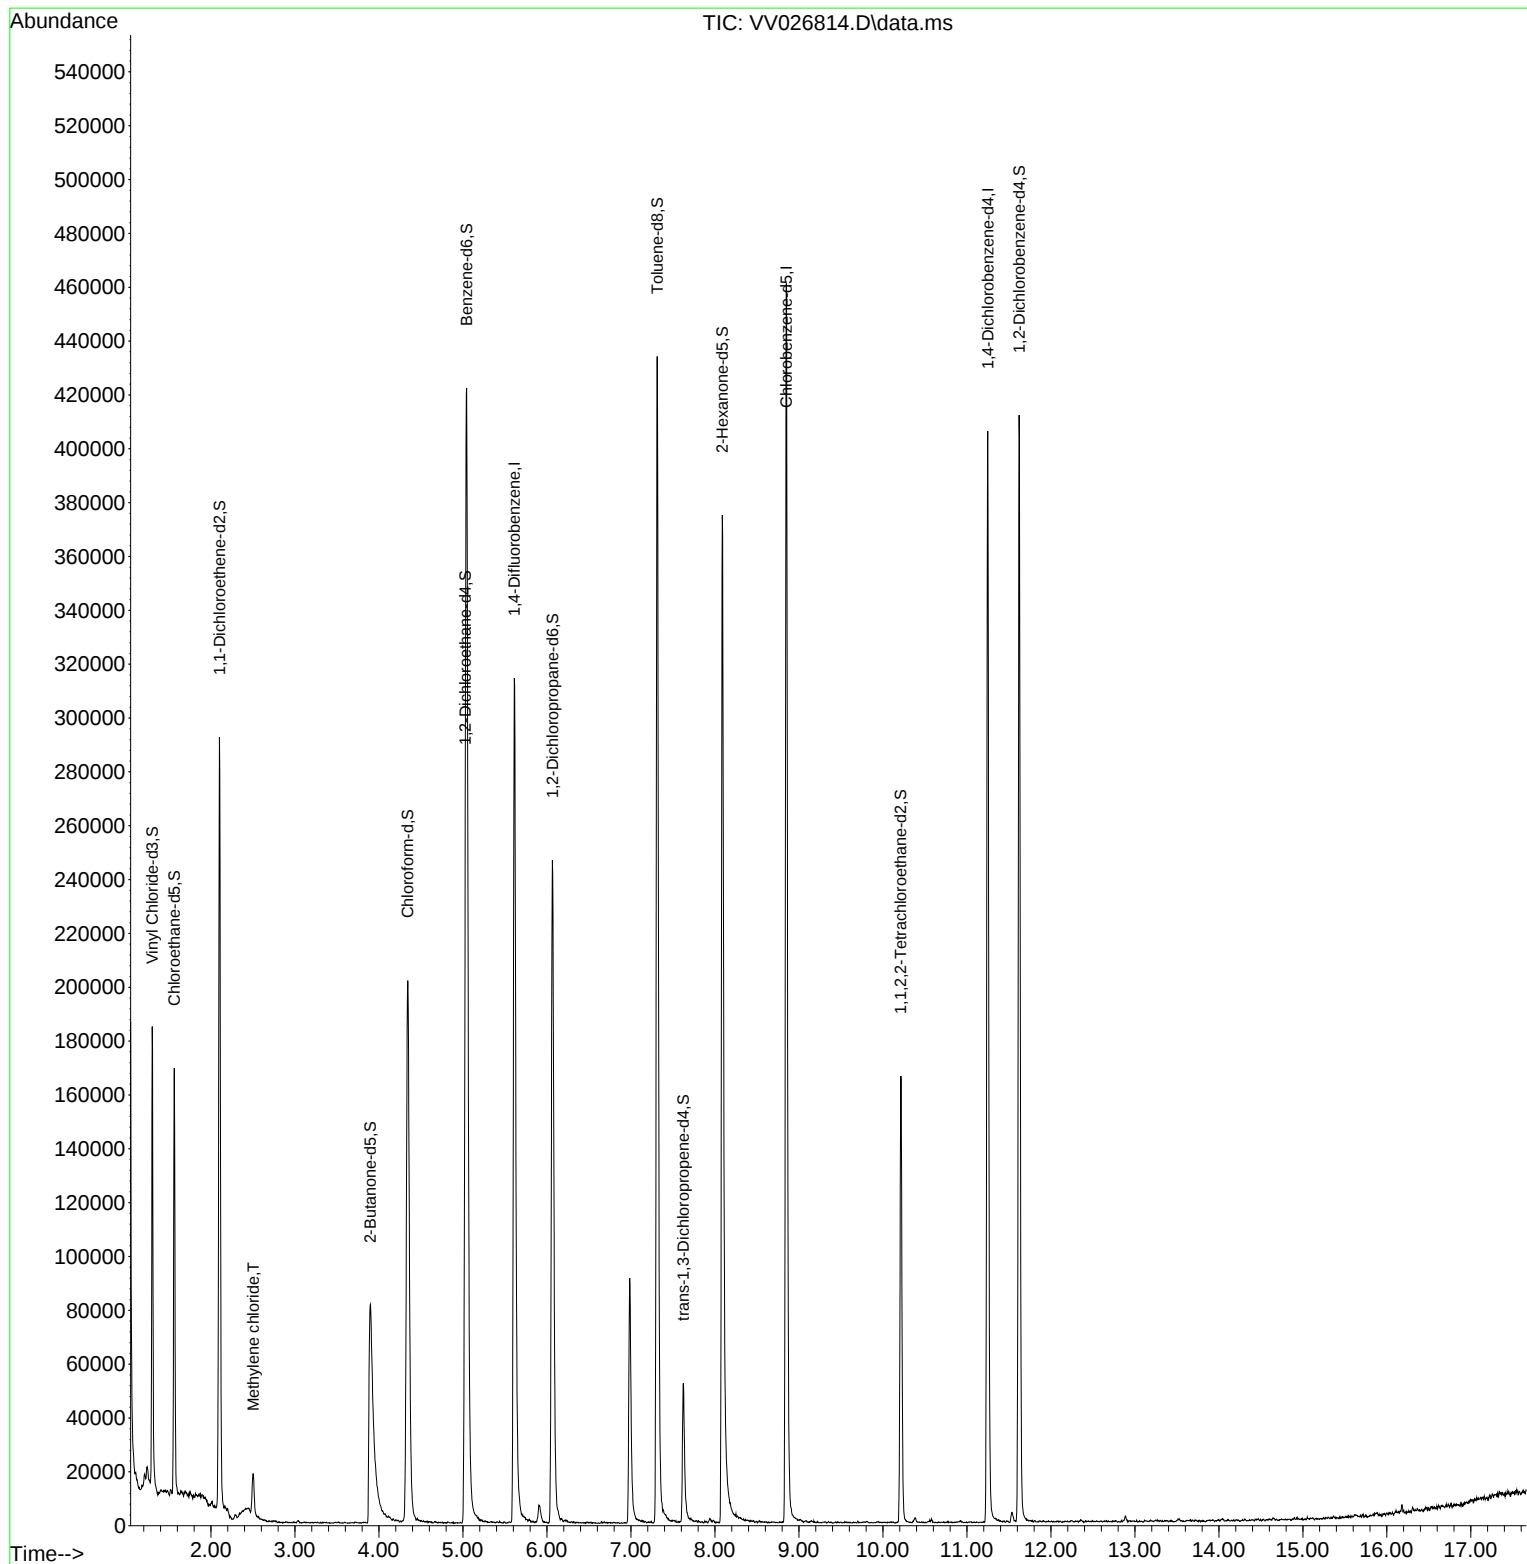

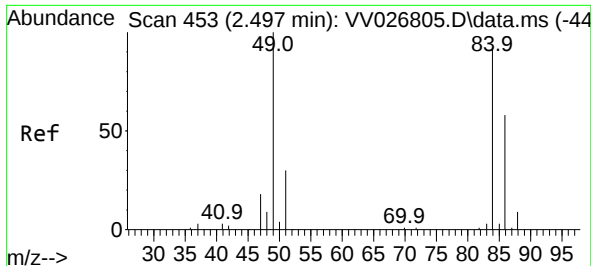

#16
Methylene chloride
Concen: 0.241 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV026814.D
Acq: 18 Jul 2022 16:32

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

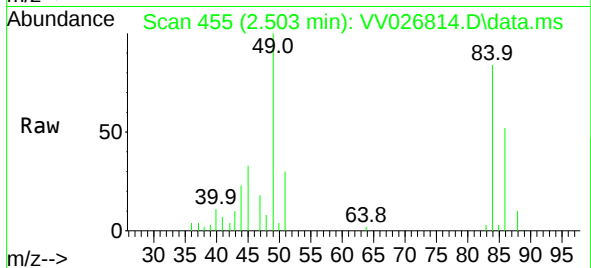

Tgt Ion: 84 Resp: 7059

Ion	Ratio	Lower	Upper
84	100		
86	61.8	44.8	83.2
49	118.7	78.7	146.1

