

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071822\
 Data File : VW026815.D
 Acq On : 18 Jul 2022 16:59
 Operator : SY/MD
 Sample : N3709-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Quant Time: Jul 19 03:11:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jul 19 03:06:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	230459	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	230803	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	96736	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	86401	4.110	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	82.200%	
7) Chloroethane-d5	1.564	69	83811	4.614	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.200%	
11) 1,1-Dichloroethene-d2	2.101	63	119397	2.958	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	59.200%#	
20) 2-Butanone-d5	3.895	46	206556	62.948	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	125.900%	
24) Chloroform-d	4.342	84	184757	5.026	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.600%	
26) 1,2-Dichloroethane-d4	5.030	65	86617	5.393	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.800%	
32) Benzene-d6	5.047	84	331411	4.725	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.600%	
36) 1,2-Dichloropropane-d6	6.066	67	112599	5.355	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	107.000%	
41) Toluene-d8	7.313	98	240329	3.860	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	77.200%	
43) trans-1,3-Dichloroprop...	7.625	79	30971	4.502	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.000%	
46) 2-Hexanone-d5	8.088	63	158767	53.302	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	106.600%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	85752	5.235	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	96593	5.731	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	114.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	9199	0.382	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026815.D
Acq On : 18 Jul 2022 16:59
Operator : SY/MD
Sample : N3709-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002


Quant Time: Jul 19 03:11:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 19 03:06:10 2022
Response via : Initial Calibration

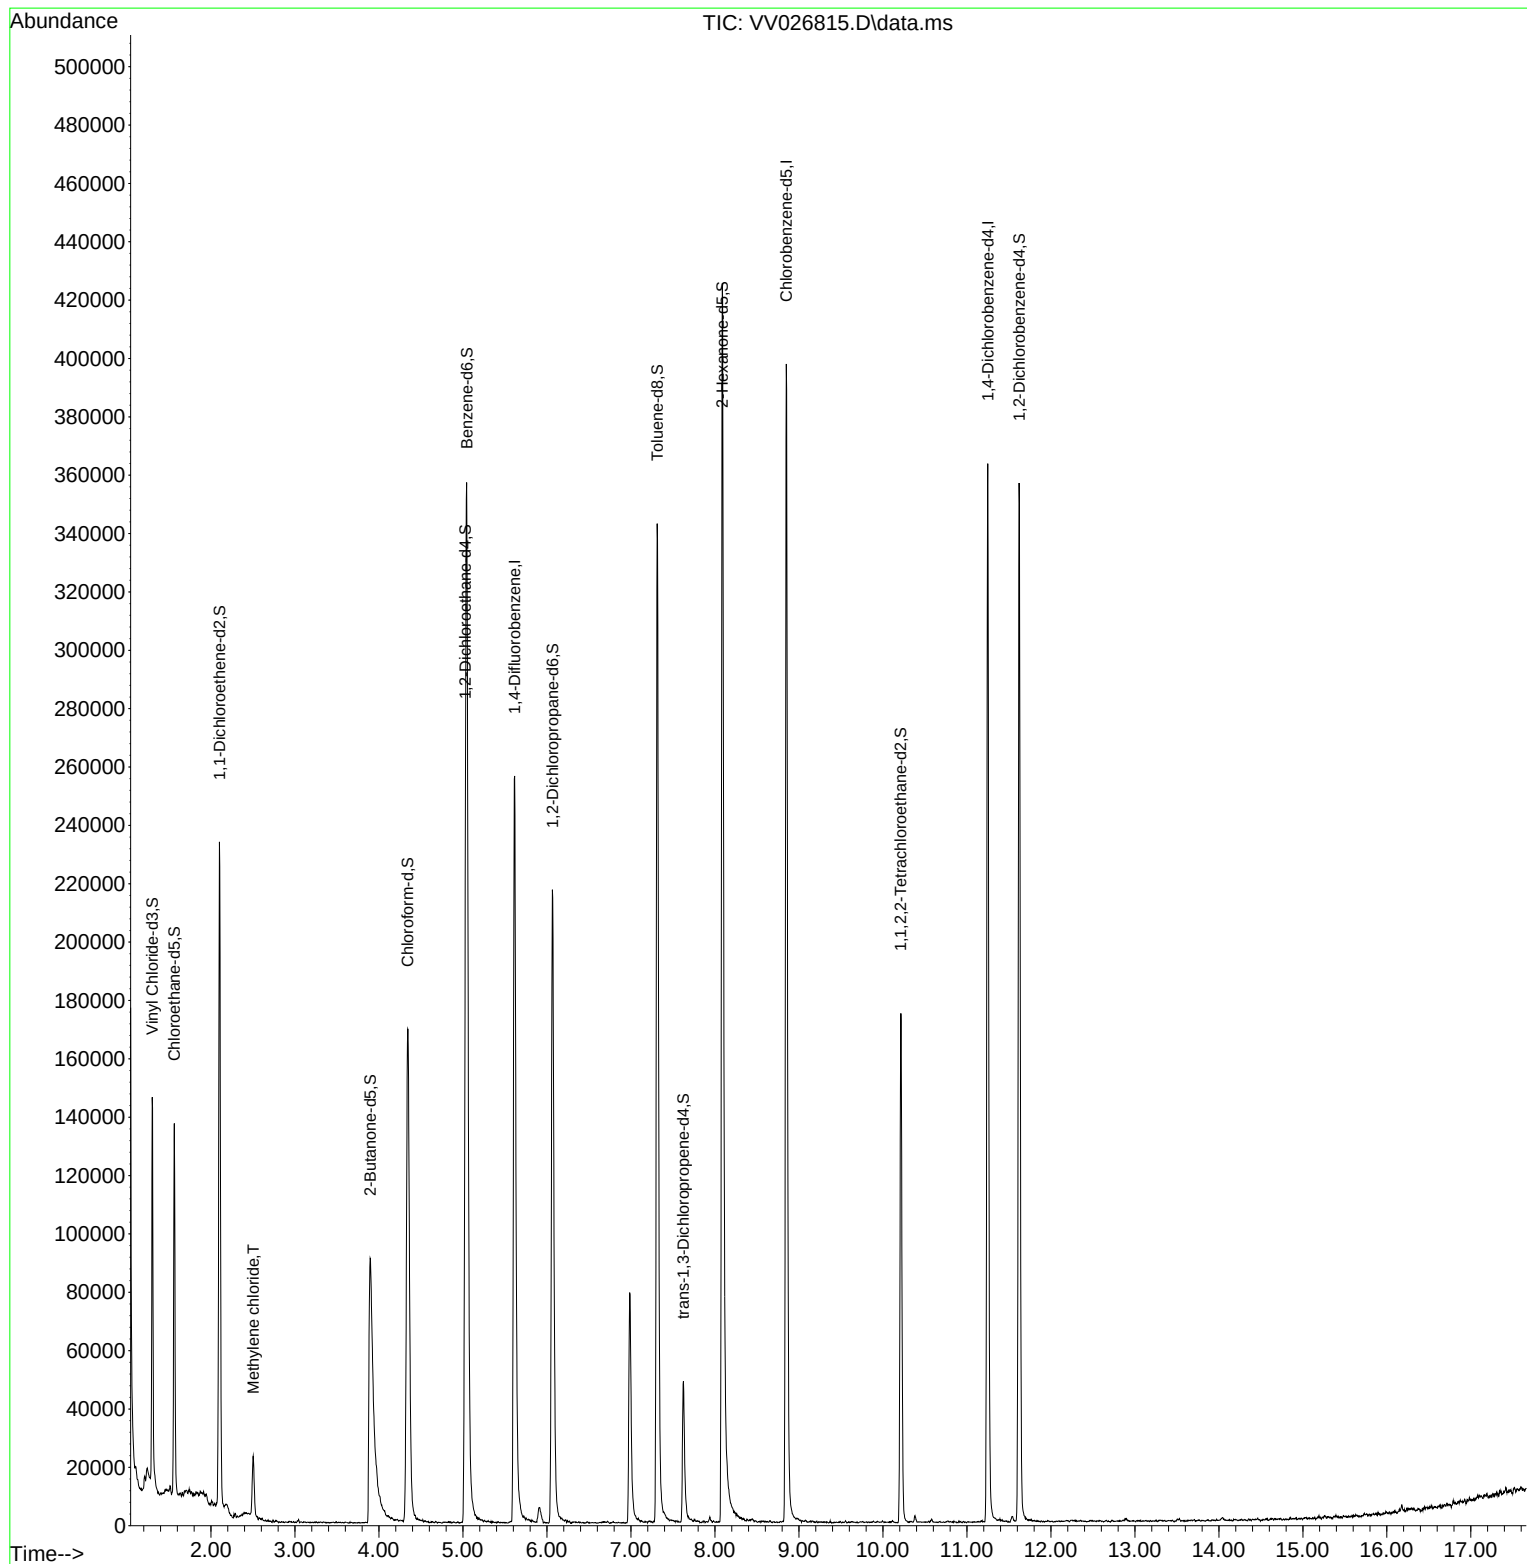

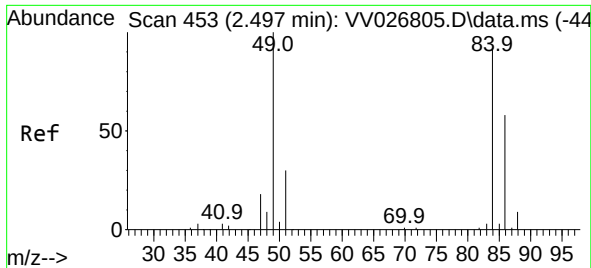

#16
Methylene chloride
Concen: 0.382 ug/L
RT: 2.503 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV026815.D
Acq: 18 Jul 2022 16:59

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

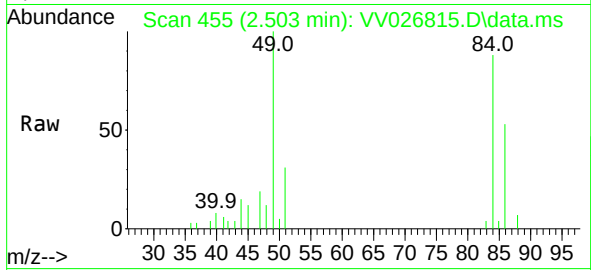

Tgt Ion: 84 Resp: 9199

Ion	Ratio	Lower	Upper
84	100		
86	61.0	44.8	83.2
49	114.2	78.7	146.1

