

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071822\
 Data File : VW026817.D
 Acq On : 18 Jul 2022 17:49
 Operator : SY/MD
 Sample : N3710-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jul 19 03:11:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jul 19 03:06:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	238476	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	240015	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	95556	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	83792	3.851	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	77.000%	
7) Chloroethane-d5	1.561	69	81769	4.350	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	87.000%	
11) 1,1-Dichloroethene-d2	2.101	63	116243	2.783	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	55.600%#	
20) 2-Butanone-d5	3.905	46	211198	62.199	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	124.400%	
24) Chloroform-d	4.346	84	186119	4.892	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.800%	
26) 1,2-Dichloroethane-d4	5.031	65	88197	5.307	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.200%	
32) Benzene-d6	5.047	84	320425	4.393	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.800%	
36) 1,2-Dichloropropane-d6	6.069	67	112875	5.162	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.200%	
41) Toluene-d8	7.317	98	234104	3.616	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	72.400%	
43) trans-1,3-Dichloroprop...	7.625	79	32076	4.483	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.600%	
46) 2-Hexanone-d5	8.091	63	158488	51.166	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	102.340%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	88125	5.173	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	92075	5.530	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	12127	0.487	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026817.D
Acq On : 18 Jul 2022 17:49
Operator : SY/MD
Sample : N3710-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jul 19 03:11:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 19 03:06:10 2022
Response via : Initial Calibration

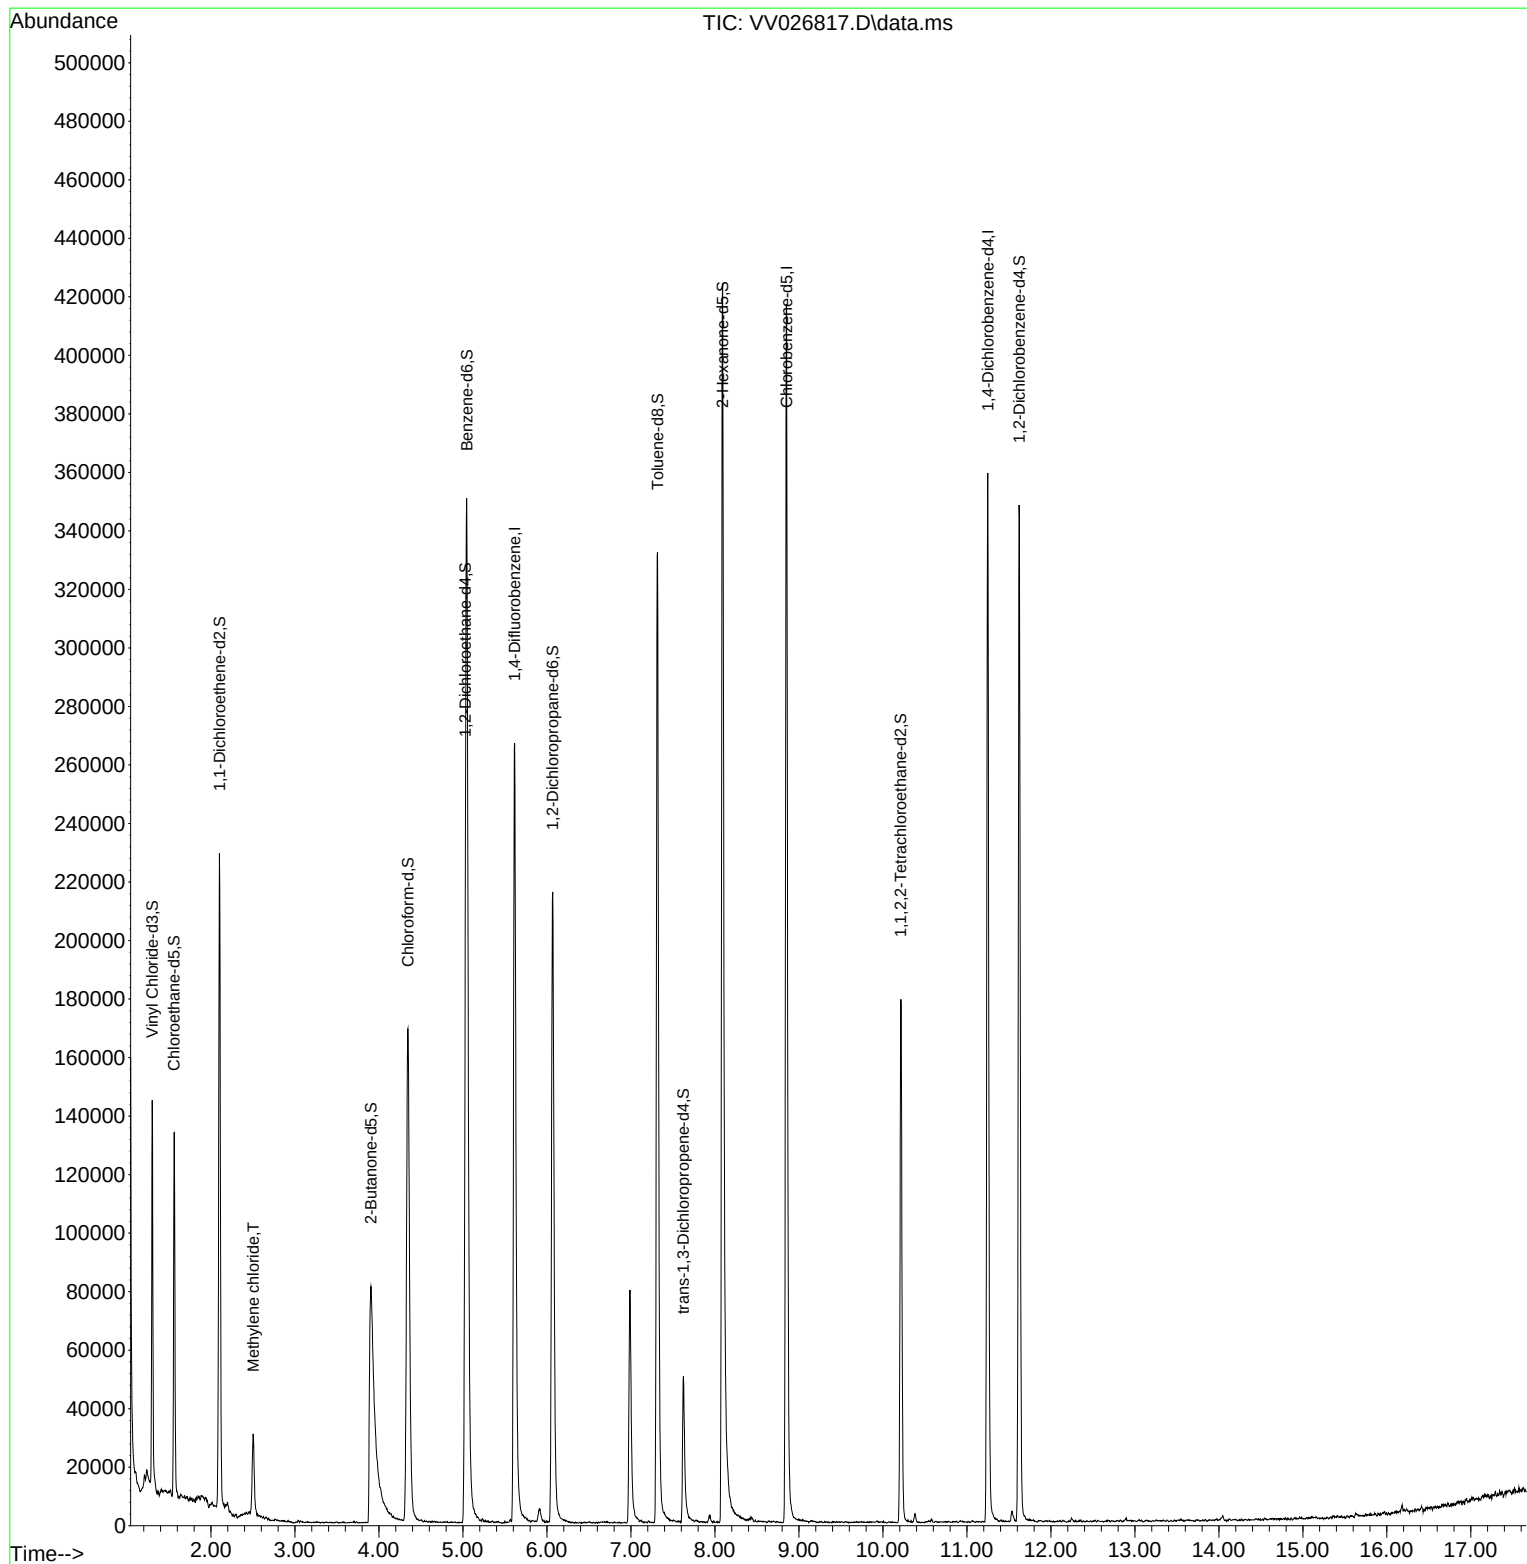

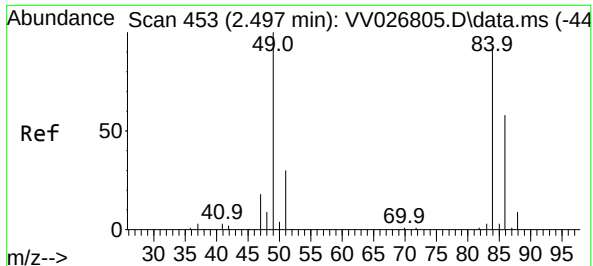

#16
Methylene chloride
Concen: 0.487 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV026817.D
Acq: 18 Jul 2022 17:49

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

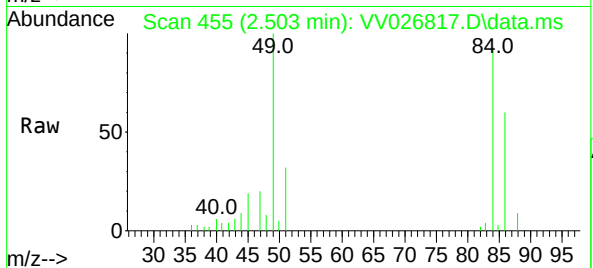

Tgt Ion: 84 Resp: 12127

Ion	Ratio	Lower	Upper
84	100		
86	64.0	44.8	83.2
49	107.4	78.7	146.1

