

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071822\
 Data File : VW026818.D
 Acq On : 18 Jul 2022 18:14
 Operator : SY/MD
 Sample : VIBLK277
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK277

Quant Time: Jul 19 03:12:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Jul 19 03:06:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	226027	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	226986	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	91402	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	82401	3.996	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.000%
7) Chloroethane-d5	1.565	69	81210	4.558	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.200%
11) 1,1-Dichloroethene-d2	2.102	63	115987	2.930	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.600%#
20) 2-Butanone-d5	3.892	46	171879	53.407	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.820%
24) Chloroform-d	4.346	84	184145	5.107	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.200%
26) 1,2-Dichloroethane-d4	5.031	65	87847	5.577	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.600%
32) Benzene-d6	5.047	84	322536	4.676	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.600%
36) 1,2-Dichloropropane-d6	6.069	67	111145	5.374	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.400%
41) Toluene-d8	7.314	98	232833	3.803	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.000%
43) trans-1,3-Dichloroprop...	7.625	79	29567	4.370	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.400%
46) 2-Hexanone-d5	8.088	63	156492	53.421	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.840%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	86407	5.363	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	90291	5.670	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.400%
Target Compounds						
16) Methylene chloride	2.503	84	12947	0.548	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026818.D
Acq On : 18 Jul 2022 18:14
Operator : SY/MD
Sample : VIBLK277
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Quant Time: Jul 19 03:12:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Jul 19 03:06:10 2022
Response via : Initial Calibration

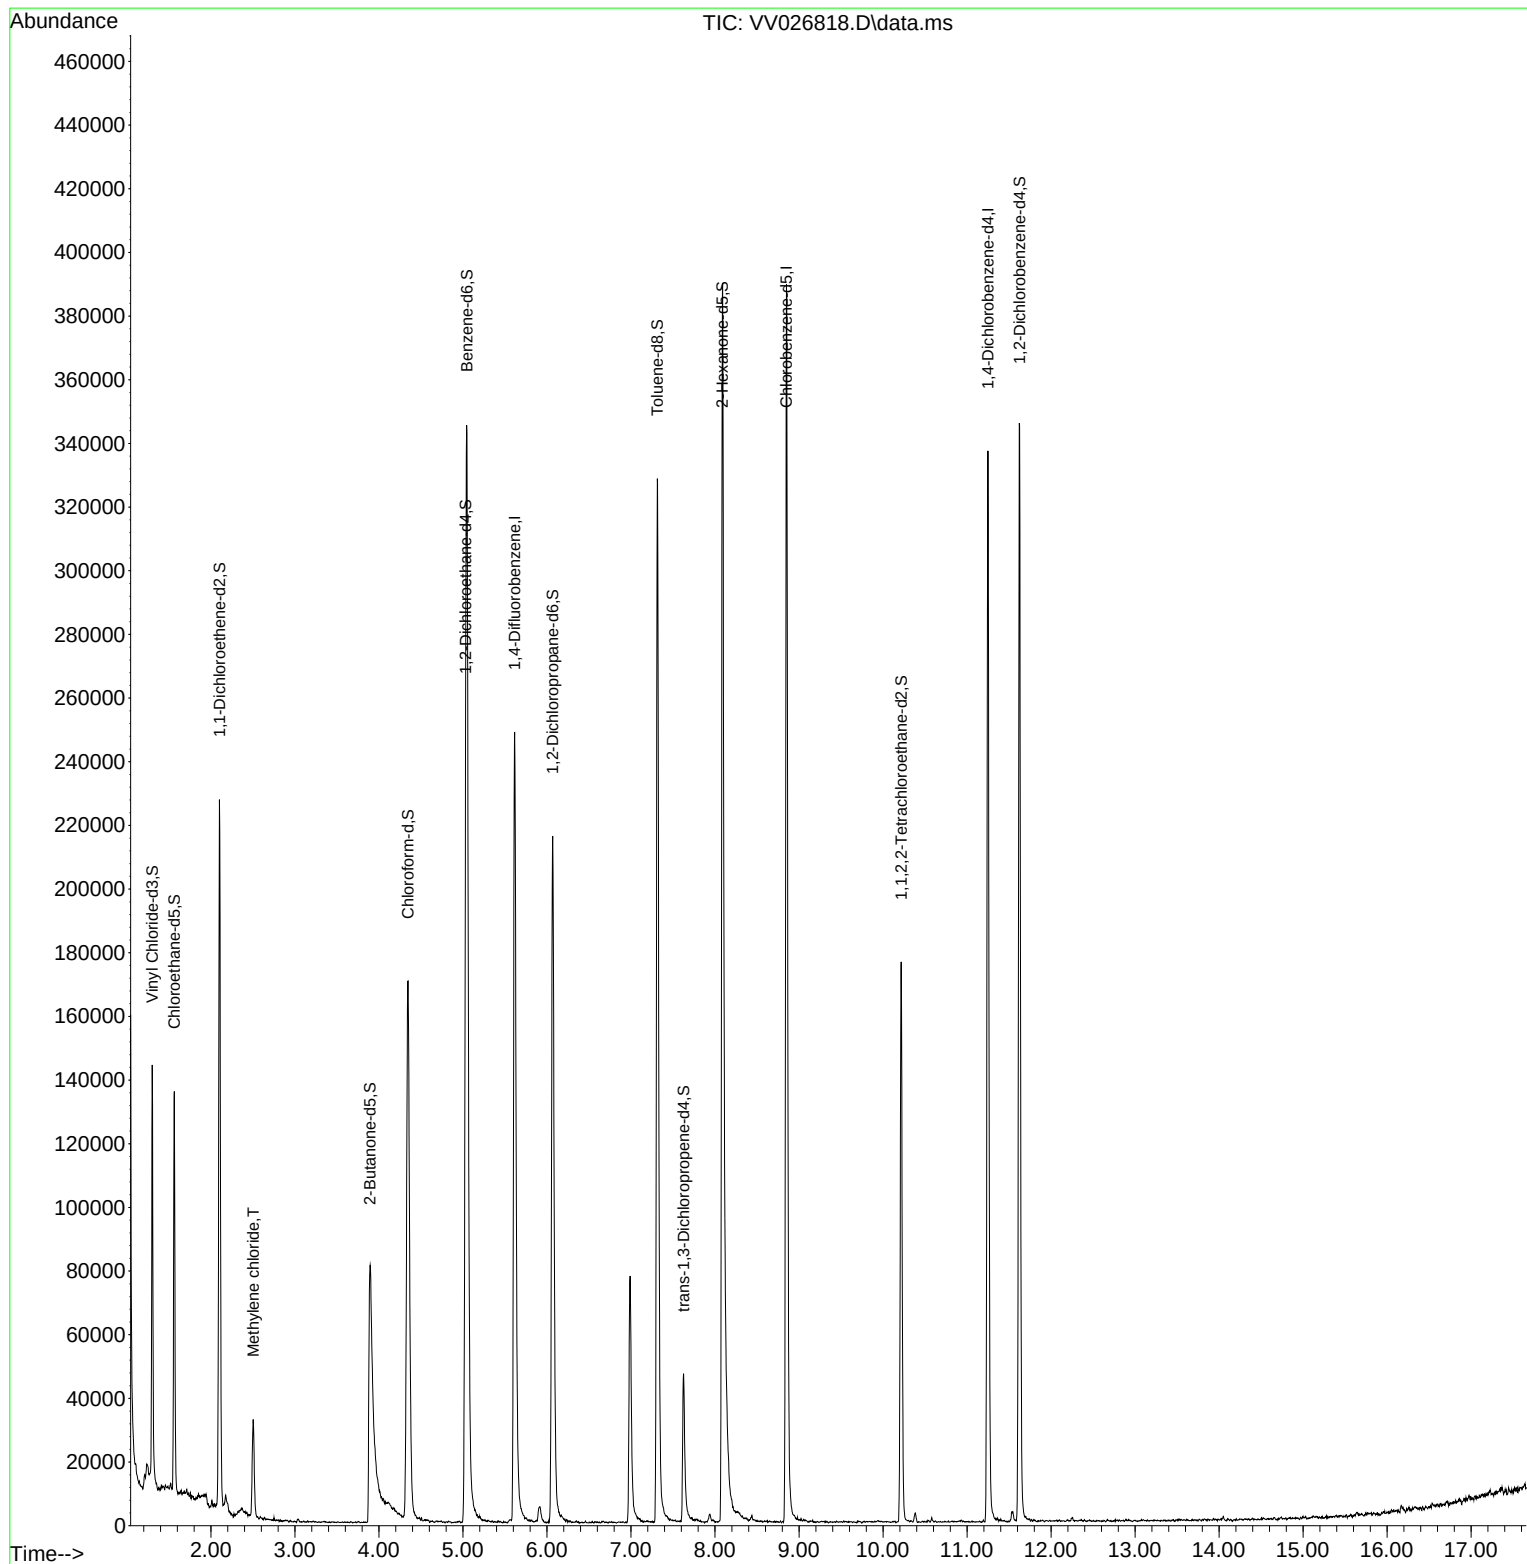

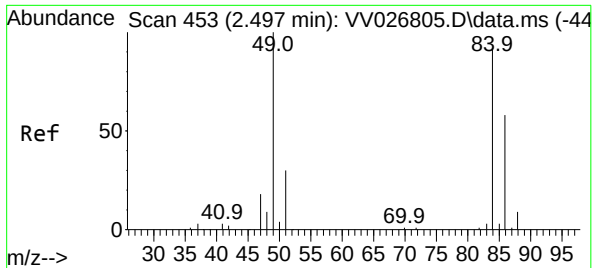

#16
Methylene chloride
Concen: 0.548 ug/L
RT: 2.503 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV026818.D
Acq: 18 Jul 2022 18:14

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Tgt Ion:	84	Resp:	12947
Ion	Ratio	Lower	Upper
84	100		
86	63.5	44.8	83.2
49	116.4	78.7	146.1

