

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
 Data File : VV026813.D
 Acq On : 18 Jul 2022 16:03
 Operator : SY/MD
 Sample : VIBLK276
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK276

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026813.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	100	rVB	138796	152882	16.98%	2.087%
2	1.564	156	163	179	rVB	127069	143365	15.93%	1.957%
3	2.105	320	331	344	rBV	232527	329494	36.60%	4.499%
4	2.503	444	455	473	rVB	54233	89894	9.99%	1.227%
5	3.892	876	887	925	rBV2	101251	344292	38.24%	4.701%
6	4.346	1011	1028	1061	rBV	166129	427021	47.43%	5.830%
7	5.043	1227	1245	1279	rBV2	360793	900245	100.00%	12.292%
8	5.616	1410	1423	1448	rBV	291043	598249	66.45%	8.168%
9	5.915	1505	1516	1528	rBV7	5004	10662	1.18%	0.146%
10	6.069	1549	1564	1589	rBV	215220	448989	49.87%	6.130%
11	6.989	1839	1850	1870	rBV	79362	152585	16.95%	2.083%
12	7.317	1939	1952	1980	rBV	352261	636196	70.67%	8.686%
13	7.625	2038	2048	2071	rBV	46730	88289	9.81%	1.205%
14	8.088	2177	2192	2226	rBV	413884	791632	87.94%	10.809%
15	8.850	2418	2429	2449	rBV	446109	739701	82.17%	10.100%
16	10.214	2838	2853	2876	rBV	166361	269602	29.95%	3.681%
17	11.249	3164	3175	3199	rBV	401070	620827	68.96%	8.477%
18	11.622	3279	3291	3308	rBV	355849	570238	63.34%	7.786%
19	16.930	4938	4942	4947	rBV	17265	9842	1.09%	0.134%




Sum of corrected areas: 7324005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026813.D
Acq On : 18 Jul 2022 16:03
Operator : SY/MD
Sample : VIBLK276
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

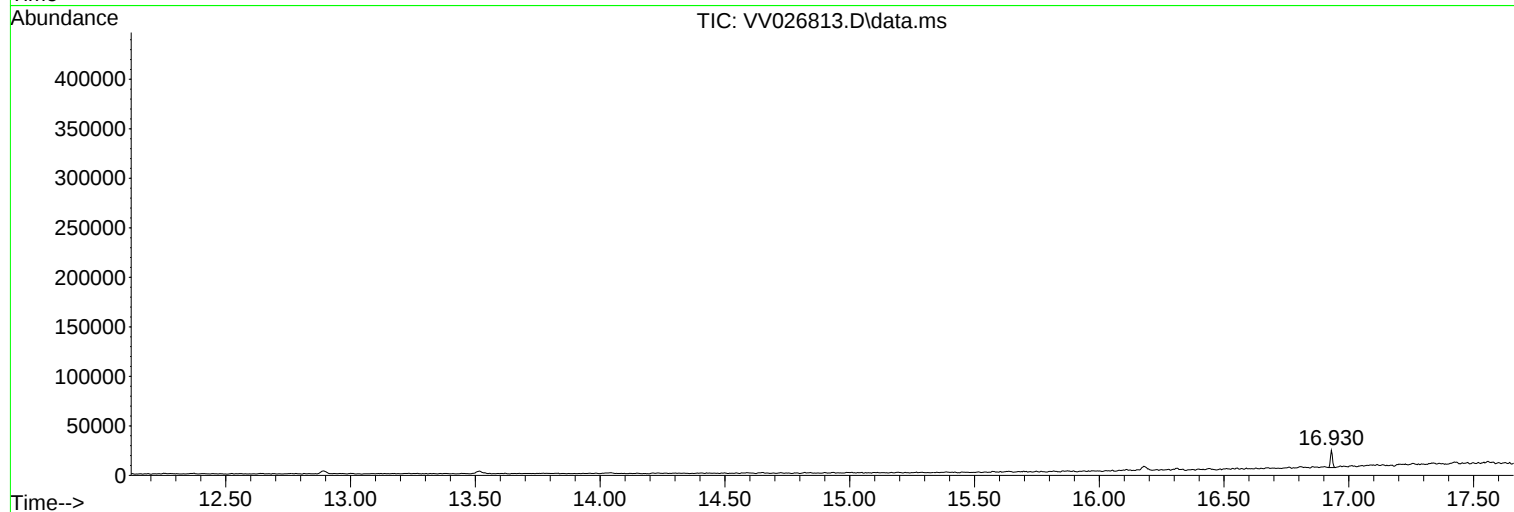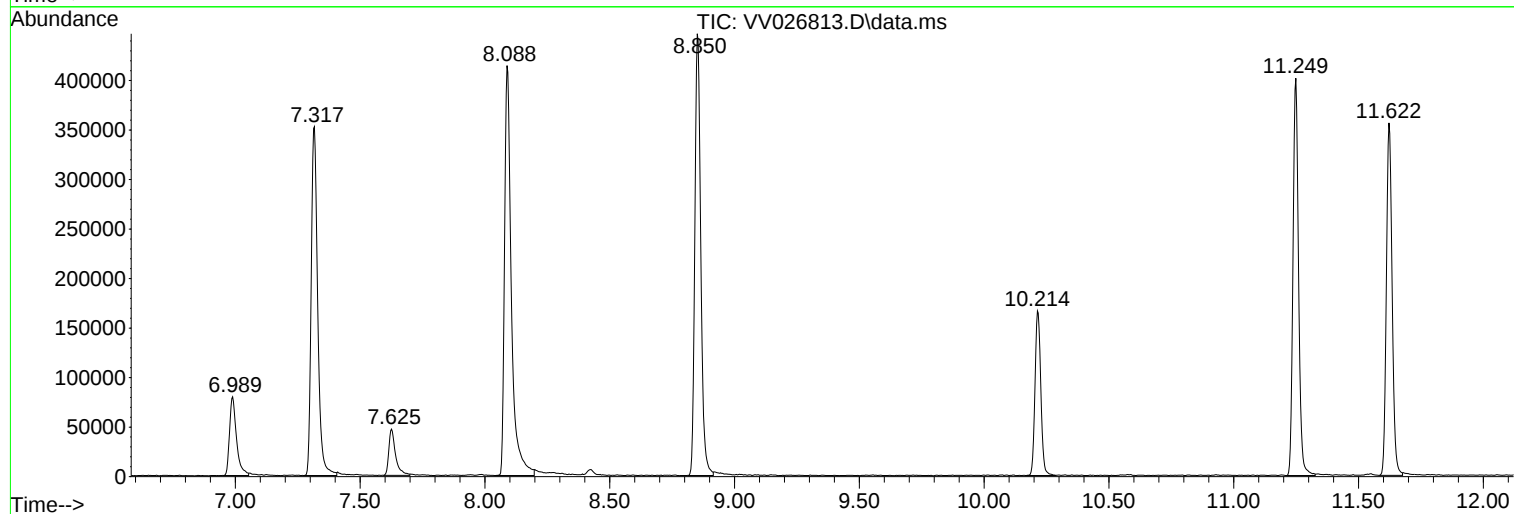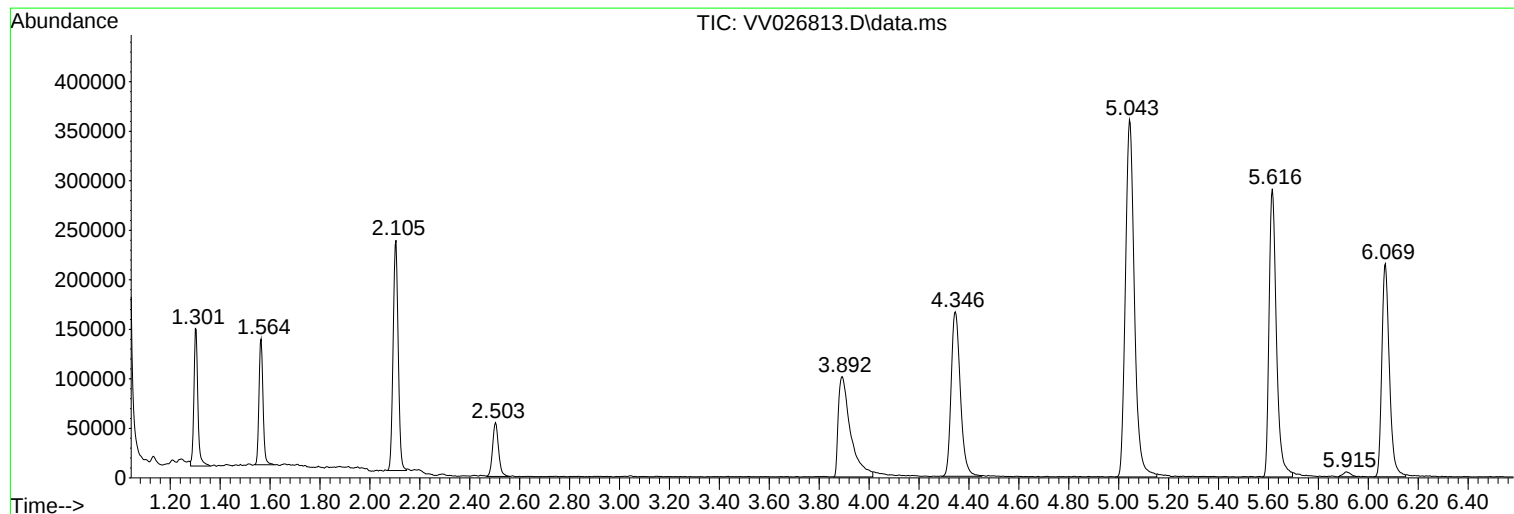

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026813.D
Acq On : 18 Jul 2022 16:03
Operator : SY/MD
Sample : VIBLK276
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026813.D
Acq On : 18 Jul 2022 16:03
Operator : SY/MD
Sample : VIBLK276
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK276

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc