

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
 Data File : VV026818.D
 Acq On : 18 Jul 2022 18:14
 Operator : SY/MD
 Sample : VIBLK277
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK277

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	95	rVB	131475	134981	15.40%	1.954%
2	1.565	155	163	176	rVB	126390	141663	16.16%	2.051%
3	2.102	320	330	343	rVB	221685	314063	35.82%	4.546%
4	2.175	349	353	365	rVB6	5286	9138	1.04%	0.132%
5	2.503	445	455	469	rVB	30674	50484	5.76%	0.731%
6	3.896	877	888	922	rBV2	80705	294910	33.64%	4.269%
7	4.346	1010	1028	1051	rBV	168504	422270	48.17%	6.113%
8	5.043	1228	1245	1282	rBV3	344769	876682	100.00%	12.691%
9	5.616	1411	1423	1460	rBV	247678	518620	59.16%	7.507%
10	5.915	1505	1516	1526	rBV6	4577	10194	1.16%	0.148%
11	6.069	1549	1564	1586	rBV	215804	450474	51.38%	6.521%
12	6.989	1838	1850	1877	rBV	77534	154179	17.59%	2.232%
13	7.314	1939	1951	1982	rBV	327895	596888	68.08%	8.640%
14	7.625	2038	2048	2074	rBV	46555	89706	10.23%	1.299%
15	8.088	2182	2192	2230	rBV	388704	828622	94.52%	11.995%
16	8.850	2418	2429	2456	rBV	388893	653058	74.49%	9.453%
17	10.217	2842	2854	2877	rBV	175940	277948	31.70%	4.023%
18	11.249	3163	3175	3202	rBV	336530	534977	61.02%	7.744%
19	11.622	3280	3291	3311	rBV	344805	549278	62.65%	7.951%




Sum of corrected areas: 6908135

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026818.D
Acq On : 18 Jul 2022 18:14
Operator : SY/MD
Sample : VIBLK277
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

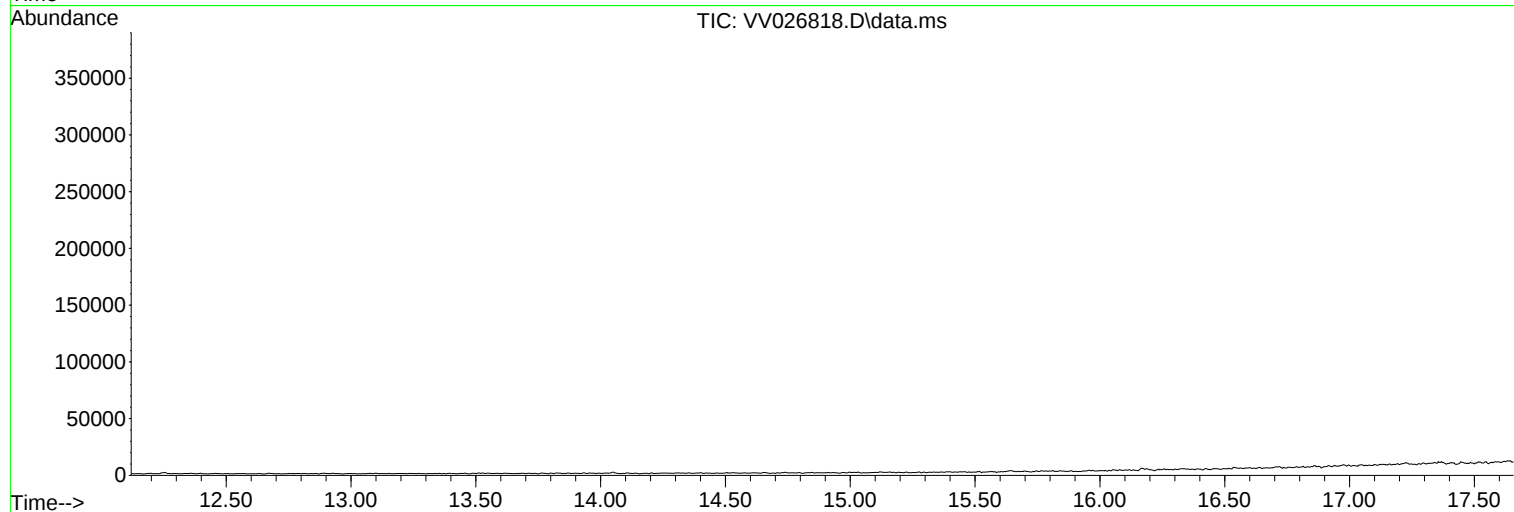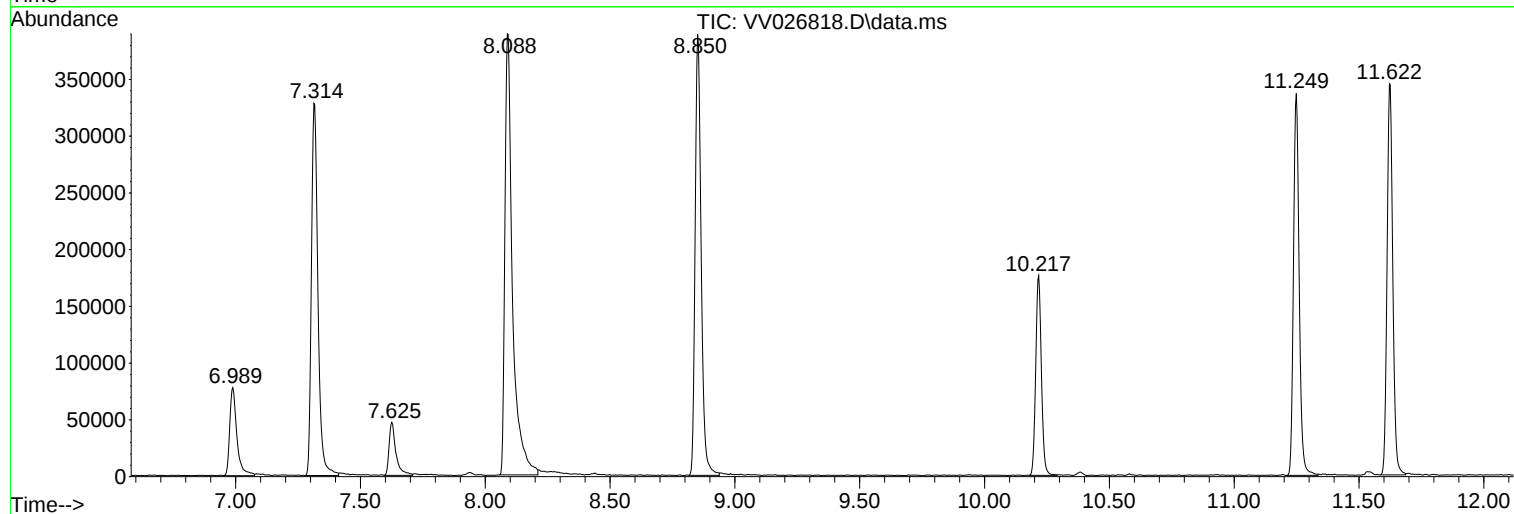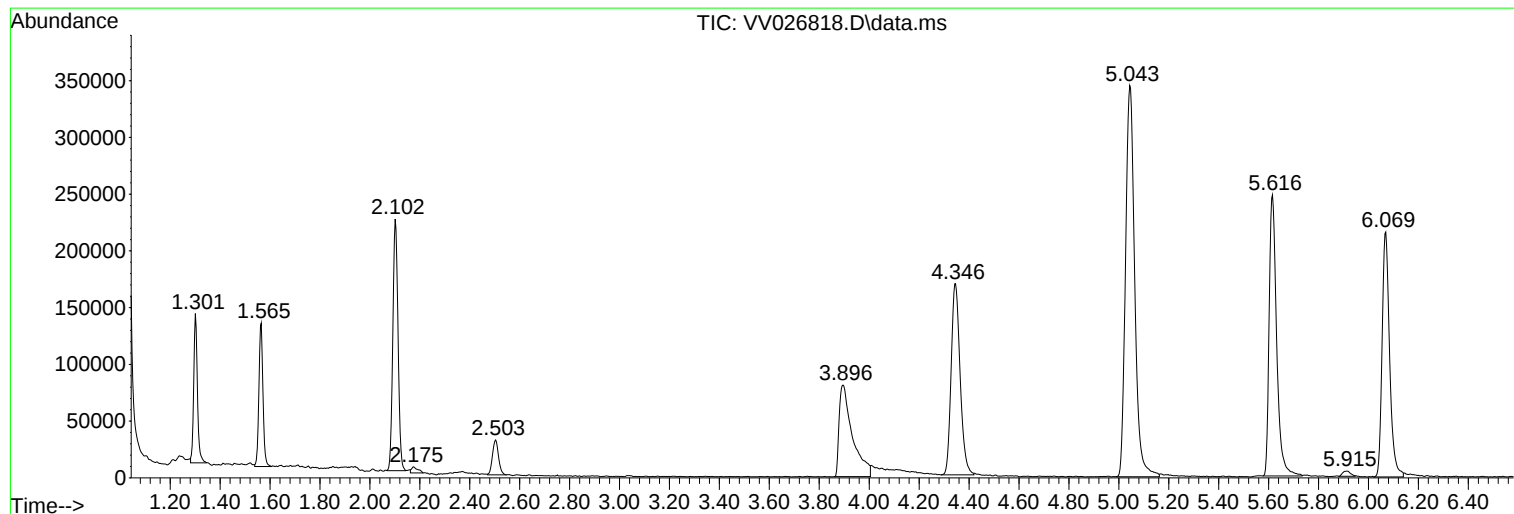

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026818.D
Acq On : 18 Jul 2022 18:14
Operator : SY/MD
Sample : VIBLK277
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071822\
Data File : VV026818.D
Acq On : 18 Jul 2022 18:14
Operator : SY/MD
Sample : VIBLK277
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc