


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV071825\
Data File : VV038914.D
Acq On : 18 Jul 2025 07:34
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\82V071125W.M
Title : SW846 8260
Last Update : Mon Jul 14 09:44:44 2025

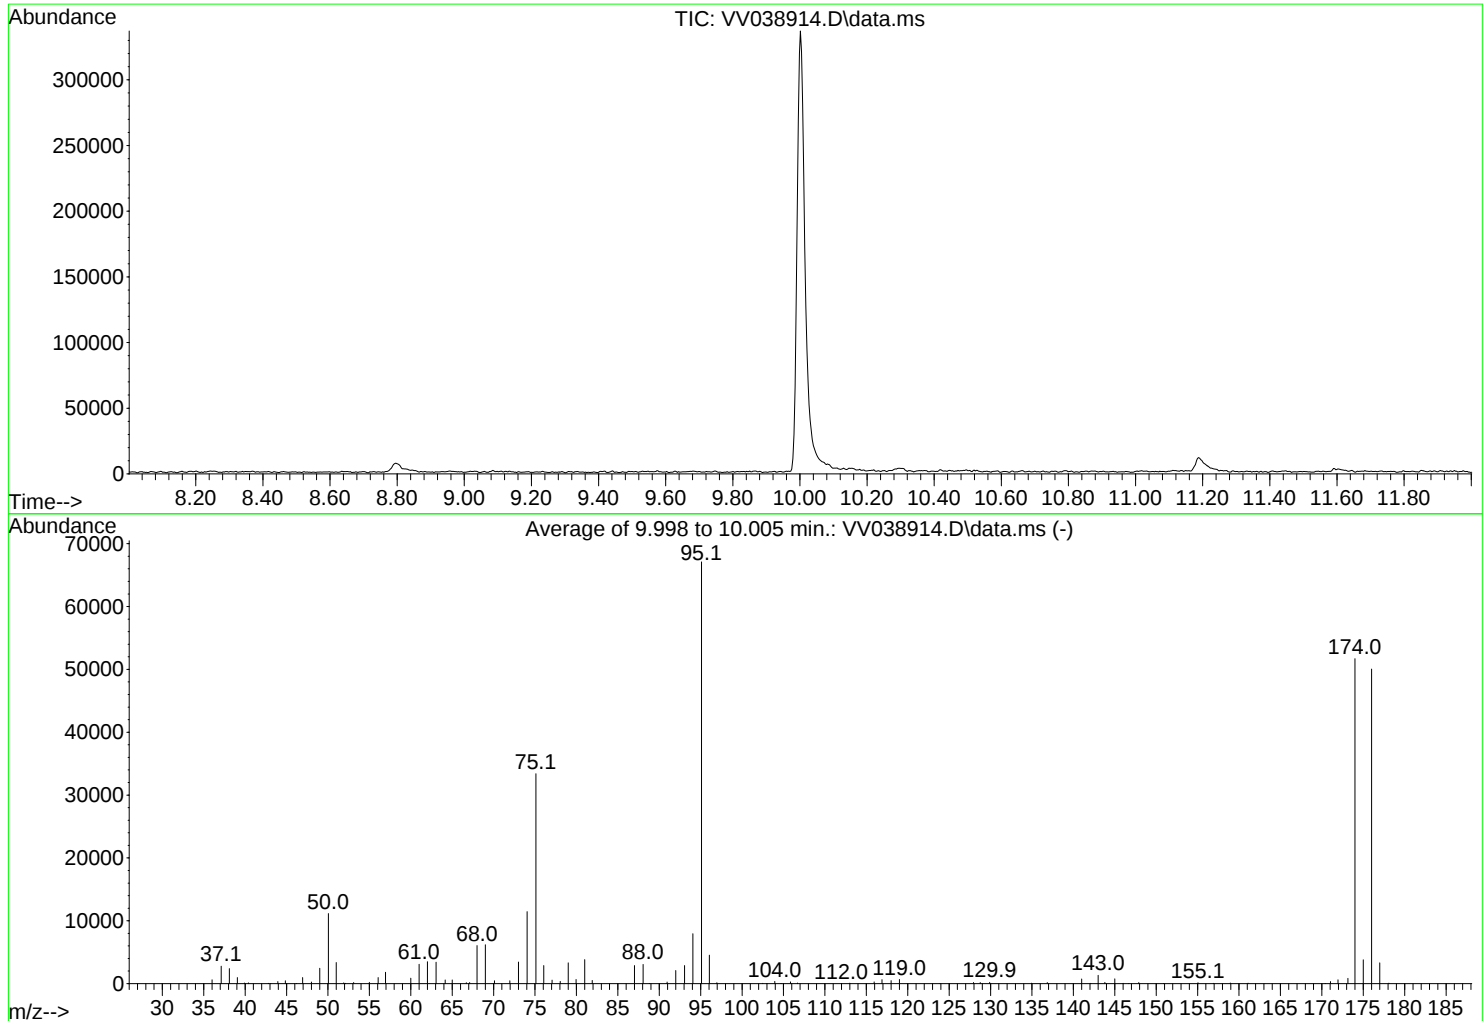

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	11141	PASS
75	95	30	60	49.8	33400	PASS
95	95	100	100	100.0	67109	PASS
96	95	5	9	6.8	4542	PASS
173	174	0.00	2	1.7	853	PASS
174	95	50	100	77.0	51696	PASS
175	174	5	9	7.3	3786	PASS
176	174	95	101	96.8	50040	PASS
177	176	5	9	6.6	3318	PASS