


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV071918\
 Data File : VV006636.D
 Acq On : 19 Jul 2018 09:09
 Operator : SY/MD
 Sample : BFB68
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB68

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jul 20 05:09:32 2018

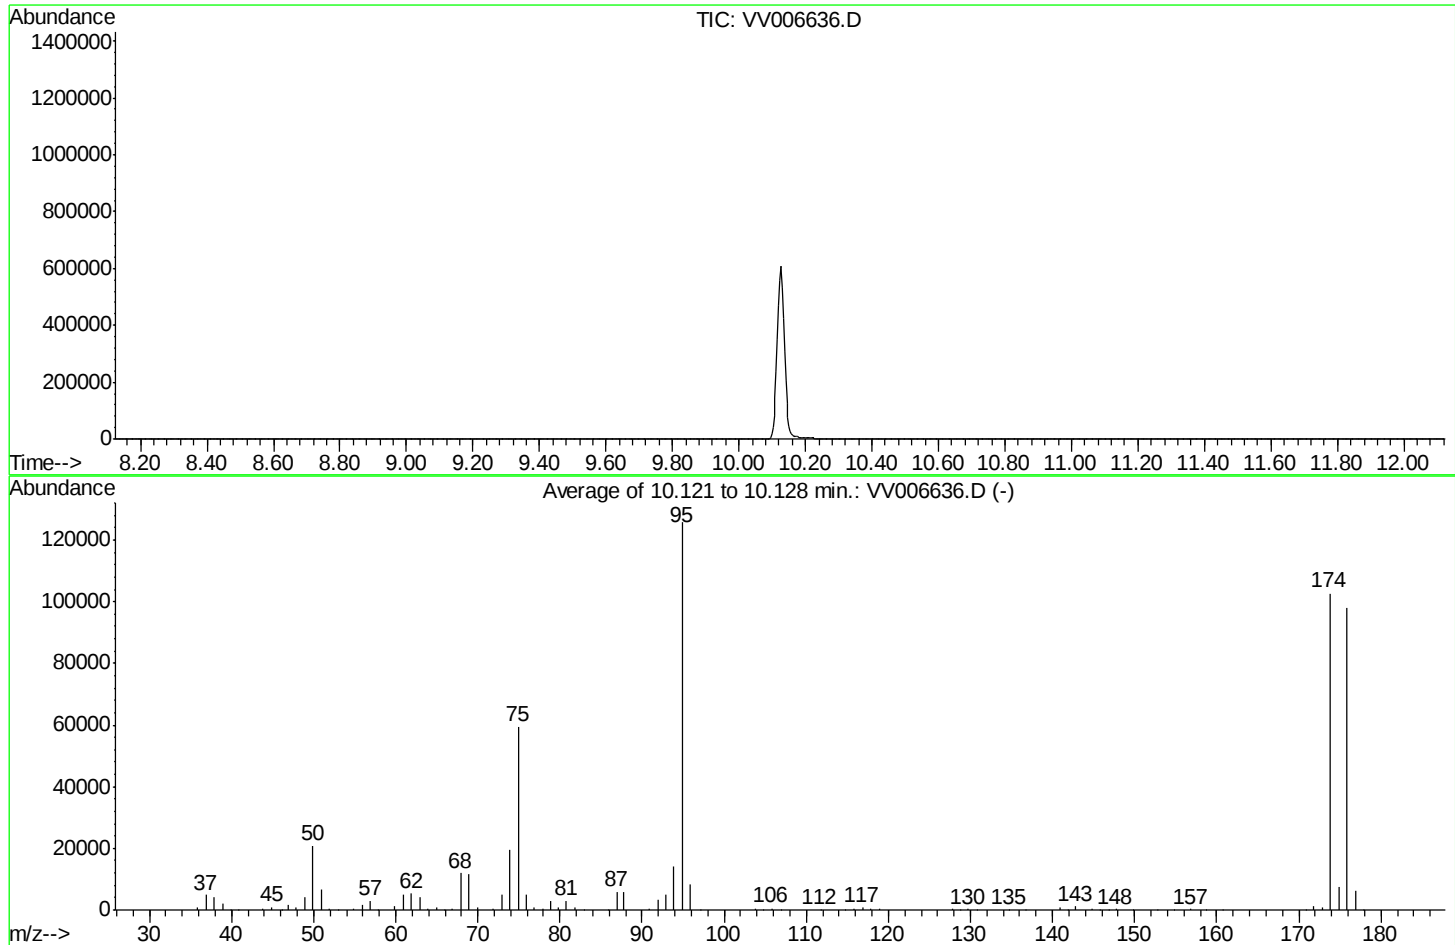

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	20826	PASS
75	95	30	80	47.4	59546	PASS
95	95	100	100	100.0	125754	PASS
96	95	5	9	6.6	8319	PASS
173	174	0.00	2	0.9	926	PASS
174	95	50	120	81.6	102640	PASS
175	174	5	9	7.1	7284	PASS
176	174	95	101	95.4	97880	PASS
177	176	5	9	6.5	6365	PASS

Scan 2858 (10.080 min): VV006636.D
BFB68

m/z	Abundance
39.80	149.0
43.80	506.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	819.0
36.90	4635.0
37.90	4326.0
38.90	1967.0
39.90	217.0
40.80	124.0
43.80	977.0
44.90	958.0
46.10	132.0
46.90	1763.0
47.90	721.0
48.90	4211.0
49.90	20232.0
50.90	6443.0
51.90	317.0
52.90	124.0
54.80	297.0
55.90	1483.0
56.90	3069.0
57.80	132.0
59.90	1120.0
60.90	4946.0
61.90	5147.0
63.00	3995.0
63.90	578.0
64.90	908.0
65.90	113.0
66.80	250.0
67.90	11261.0
68.90	11357.0
69.90	696.0
71.80	606.0
72.90	4785.0
73.90	18744.0
74.90	57752.0
75.90	4819.0
76.80	967.0
77.80	528.0
78.80	2828.0
79.90	947.0
80.80	2970.0
81.80	664.0
85.90	158.0
86.90	5630.0
87.80	5395.0
90.90	400.0
91.90	3131.0
92.90	4846.0
93.90	13563.0
94.90	120408.0
95.90	8099.0
97.00	204.0
103.80	461.0
104.80	161.0
105.80	442.0
111.70	109.0
114.70	119.0
115.80	403.0
116.90	600.0
117.90	374.0
118.90	592.0
127.80	314.0
128.80	201.0
129.70	341.0
130.80	126.0
134.80	203.0
136.80	124.0
140.90	915.0
142.80	957.0
144.80	270.0
145.70	137.0
147.70	258.0
149.80	111.0
152.80	103.0
154.80	199.0
156.90	209.0
158.80	140.0
160.60	146.0
170.90	114.0
171.80	1165.0
172.80	861.0
173.80	95672.0
174.90	7045.0
175.80	90664.0
176.90	6084.0
177.90	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	823.0
36.90	5013.0
37.90	4445.0
38.90	2030.0
39.90	227.0
40.80	124.0
43.90	1053.0
44.90	986.0
46.10	116.0
46.90	1726.0
47.90	798.0
48.90	4500.0
49.90	21416.0
50.90	6886.0
51.90	289.0
52.90	147.0
54.80	303.0
55.90	1522.0
56.90	3235.0
57.90	145.0
59.90	1086.0
60.90	5202.0
61.90	5525.0
62.90	4290.0
63.90	596.0
64.90	931.0
65.90	112.0
66.80	301.0
67.90	12264.0
68.90	12191.0
69.90	772.0
71.80	605.0
72.90	5298.0
73.90	19976.0
74.90	61600.0
75.90	5005.0
76.80	965.0
77.90	559.0
78.80	3060.0
79.80	1048.0
80.80	3227.0
81.80	740.0
82.90	106.0
85.90	185.0
86.90	6140.0
87.80	5829.0
90.80	375.0
91.90	3418.0
92.90	5331.0
93.90	14607.0
94.90	130120.0
95.90	8572.0
97.10	221.0
103.80	516.0
104.80	196.0
105.80	497.0
106.90	101.0
111.70	108.0
114.80	119.0
115.90	446.0
116.80	699.0
117.90	401.0
118.90	619.0
127.80	340.0
128.80	224.0
129.80	347.0
130.70	124.0
134.80	231.0
136.70	147.0
140.90	991.0
141.80	108.0
142.80	1103.0
144.80	305.0
145.70	145.0
146.80	110.0
147.80	296.0
149.80	130.0
152.80	101.0
154.70	230.0
156.80	241.0
158.70	138.0
160.70	184.0
170.90	134.0
171.80	1250.0
172.90	940.0
173.80	106272.0
174.90	7546.0
175.80	100952.0
176.90	6565.0
177.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	833.0
36.90	4844.0
37.90	4209.0
38.90	1887.0
39.80	246.0
40.70	117.0
43.90	1067.0
44.90	882.0
46.90	1542.0
47.90	777.0
48.90	4383.0
49.90	20832.0
50.90	6620.0
51.90	270.0
52.90	133.0
54.80	271.0
55.90	1420.0
56.90	3074.0
57.90	132.0
59.80	965.0
60.90	5121.0
61.90	5368.0
62.90	4214.0
63.90	573.0
65.00	897.0
66.80	335.0
67.90	12136.0
68.90	11913.0
69.90	773.0
71.90	583.0
72.90	5197.0
73.90	19440.0
74.90	59288.0
75.90	4908.0
76.80	834.0
77.90	563.0
78.80	2998.0
79.80	1065.0
80.80	3063.0
81.80	710.0
82.90	129.0
85.80	180.0
86.90	6155.0
87.80	5652.0
90.80	321.0
91.90	3296.0
92.90	5177.0
93.90	14599.0
94.90	126736.0
95.90	8288.0
97.10	199.0
103.80	468.0
104.80	202.0
105.80	512.0
106.90	107.0
114.80	126.0
115.90	421.0
116.80	742.0
117.80	404.0
118.90	635.0
127.80	338.0
128.80	213.0
129.70	337.0
130.70	129.0
134.70	228.0
136.70	168.0
140.80	969.0
141.80	116.0
142.80	1144.0
144.80	279.0
145.70	147.0
146.80	109.0
147.80	310.0
149.70	135.0
154.80	229.0
156.80	256.0
158.70	120.0
160.70	164.0
170.90	118.0
171.80	1234.0
172.90	979.0
173.80	105976.0
174.90	7261.0
175.80	102024.0
176.90	6446.0
177.80	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68