


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071921\
Data File : VV021674.D
Acq On : 19 Jul 2021 11:29
Operator : SY/MD
Sample : BFB207
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB207

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071921WMA.M
Title : VOC Analysis
Last Update : Fri Jul 23 01:17:03 2021

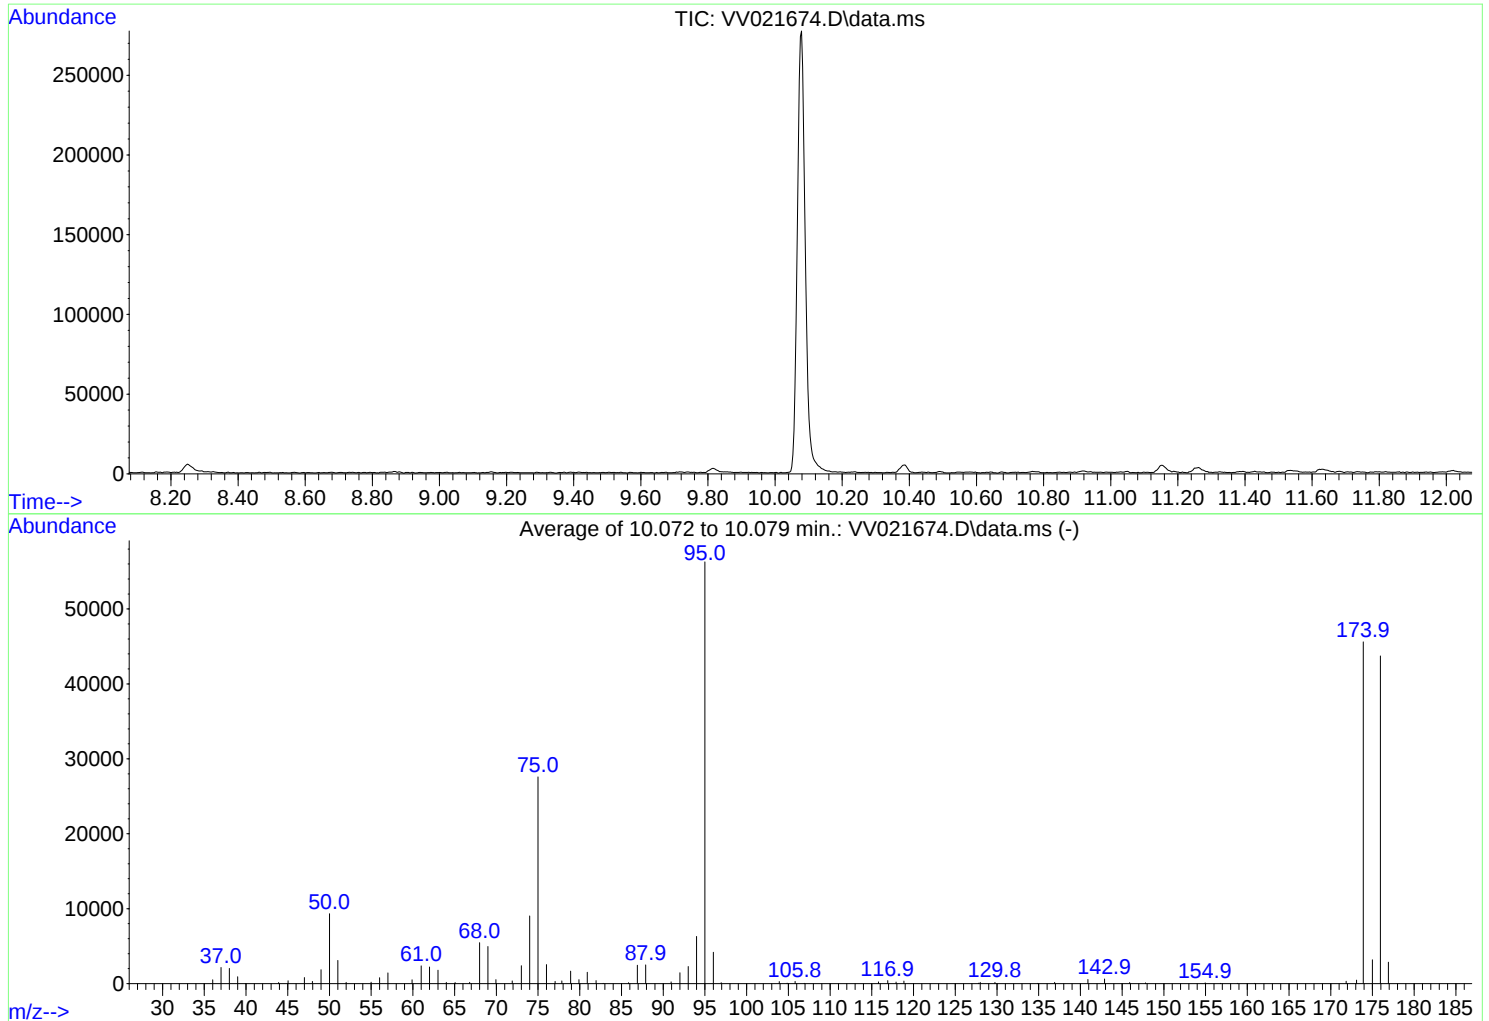

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	9331	PASS
75	95	30	80	49.0	27589	PASS
95	95	100	100	100.0	56288	PASS
96	95	5	9	7.4	4189	PASS
173	174	0.00	2	1.0	466	PASS
174	95	50	120	81.0	45619	PASS
175	174	5	9	7.0	3191	PASS
176	174	95	105	95.9	43739	PASS
177	176	5	10	6.6	2869	PASS

m/z	Abundance
40.00	196.0
42.80	123.0
43.90	489.0
76.70	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	480.0
37.00	2096.0
38.00	1876.0
39.00	822.0
40.00	244.0
43.90	582.0
45.10	328.0
47.00	731.0
48.00	269.0
49.00	1684.0
50.00	8736.0
51.00	3091.0
52.00	173.0
55.00	172.0
56.00	699.0
57.00	1285.0
59.90	456.0
61.00	2224.0
62.00	2234.0
63.00	1679.0
64.00	183.0
65.10	139.0
66.80	172.0
68.00	5269.0
69.00	4767.0
70.00	524.0
71.90	281.0
73.00	2345.0
74.00	8626.0
75.00	26176.0
76.00	2369.0
77.10	294.0
77.80	383.0
78.90	1462.0
79.90	482.0
80.90	1437.0
81.90	361.0
82.80	102.0
85.90	129.0
86.90	2197.0
87.90	2291.0
90.90	210.0
92.00	1316.0
93.00	2184.0
94.00	5816.0
95.00	53008.0
96.00	3901.0
97.10	106.0
104.00	233.0
104.90	110.0
105.80	247.0
106.90	101.0
115.90	212.0
116.90	368.0
117.90	199.0
118.90	329.0
127.80	200.0
129.80	201.0
136.90	110.0
140.90	477.0
142.90	514.0
145.90	112.0
154.90	105.0
171.80	294.0
173.10	420.0
173.90	41184.0
175.00	2901.0
175.90	39488.0
176.90	2688.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	536.0
37.00	2187.0
38.00	2144.0
39.00	958.0
39.90	216.0
43.90	636.0
45.00	393.0
47.00	848.0
48.00	303.0
49.00	1871.0
50.00	9721.0
51.00	3151.0
52.00	185.0
55.00	203.0
56.00	806.0
57.00	1461.0
59.90	535.0
61.00	2413.0
62.00	2308.0
63.00	1825.0
64.00	189.0
65.00	144.0
66.80	191.0
68.00	5650.0
69.00	5106.0
70.00	550.0
71.90	369.0
73.00	2439.0
74.00	9321.0
75.00	28648.0
76.00	2677.0
77.10	310.0
77.80	389.0
78.90	1719.0
79.90	552.0
80.90	1542.0
82.00	413.0
85.90	147.0
86.90	2535.0
87.90	2592.0
91.00	241.0
92.00	1508.0
93.00	2314.0
94.00	6507.0
95.00	57960.0
96.00	4392.0
96.90	114.0
103.90	277.0
104.80	105.0
105.80	316.0
115.80	244.0
116.90	402.0
117.90	219.0
118.80	339.0
128.00	249.0
129.80	172.0
136.90	199.0
140.90	572.0
142.90	604.0
145.90	158.0
147.80	126.0
154.90	116.0
171.80	344.0
173.10	471.0
173.90	46904.0
175.00	3295.0
175.90	44912.0
176.90	2952.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	552.0
37.00	2214.0
38.00	2091.0
39.00	977.0
39.90	203.0
43.90	733.0
45.00	430.0
47.00	869.0
47.90	330.0
49.00	1999.0
50.00	9535.0
51.00	3059.0
52.00	160.0
55.00	221.0
56.00	882.0
57.00	1542.0
59.90	563.0
61.00	2462.0
62.00	2120.0
63.00	1848.0
64.00	156.0
65.00	152.0
66.80	187.0
68.00	5505.0
69.00	5007.0
69.90	530.0
71.90	428.0
73.00	2416.0
74.00	9178.0
75.00	27944.0
76.00	2609.0
77.00	314.0
77.90	315.0
78.90	1817.0
79.90	594.0
80.90	1566.0
81.90	426.0
85.80	125.0
86.90	2605.0
87.90	2586.0
91.00	238.0
92.00	1556.0
93.00	2331.0
94.00	6559.0
95.00	57896.0
96.00	4274.0
96.90	146.0
103.80	300.0
105.80	326.0
115.70	257.0
116.90	427.0
117.90	198.0
118.80	357.0
128.00	278.0
129.70	158.0
134.90	122.0
136.90	223.0
140.90	617.0
142.90	714.0
145.90	172.0
147.80	169.0
155.00	105.0
156.80	103.0
158.80	101.0
160.90	109.0
171.90	325.0
173.10	506.0
173.90	48768.0
175.00	3378.0
176.00	46816.0
176.90	2967.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207