

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
 Data File : VV026822.D
 Acq On : 19 Jul 2022 12:38
 Operator : SY/MD
 Sample : VV0719WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK397

Quant Time: Jul 20 05:48:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 20 05:46:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	198474	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	209411	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	84005	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	98763	5.455	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.000%
7) Chloroethane-d5	1.564	69	89245	5.704	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.000%
11) 1,1-Dichloroethene-d2	2.101	63	141065	4.058	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.200%
20) 2-Butanone-d5	3.895	46	106658	37.742	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	75.480%
24) Chloroform-d	4.342	84	177665	5.611	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.200%
26) 1,2-Dichloroethane-d4	5.027	65	76662	5.543	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.800%
32) Benzene-d6	5.043	84	325179	5.110	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.200%
36) 1,2-Dichloropropane-d6	6.066	67	103381	5.419	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.400%
41) Toluene-d8	7.313	98	244347	4.326	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.600%
43) trans-1,3-Dichloroprop...	7.622	79	26901	4.310	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.200%
46) 2-Hexanone-d5	8.088	63	111411	41.224	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.440%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	73845	4.968	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	81673	5.580	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.600%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	18465	0.891	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026822.D
Acq On : 19 Jul 2022 12:38
Operator : SY/MD
Sample : VV0719WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK397


Quant Time: Jul 20 05:48:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 20 05:46:20 2022
Response via : Initial Calibration

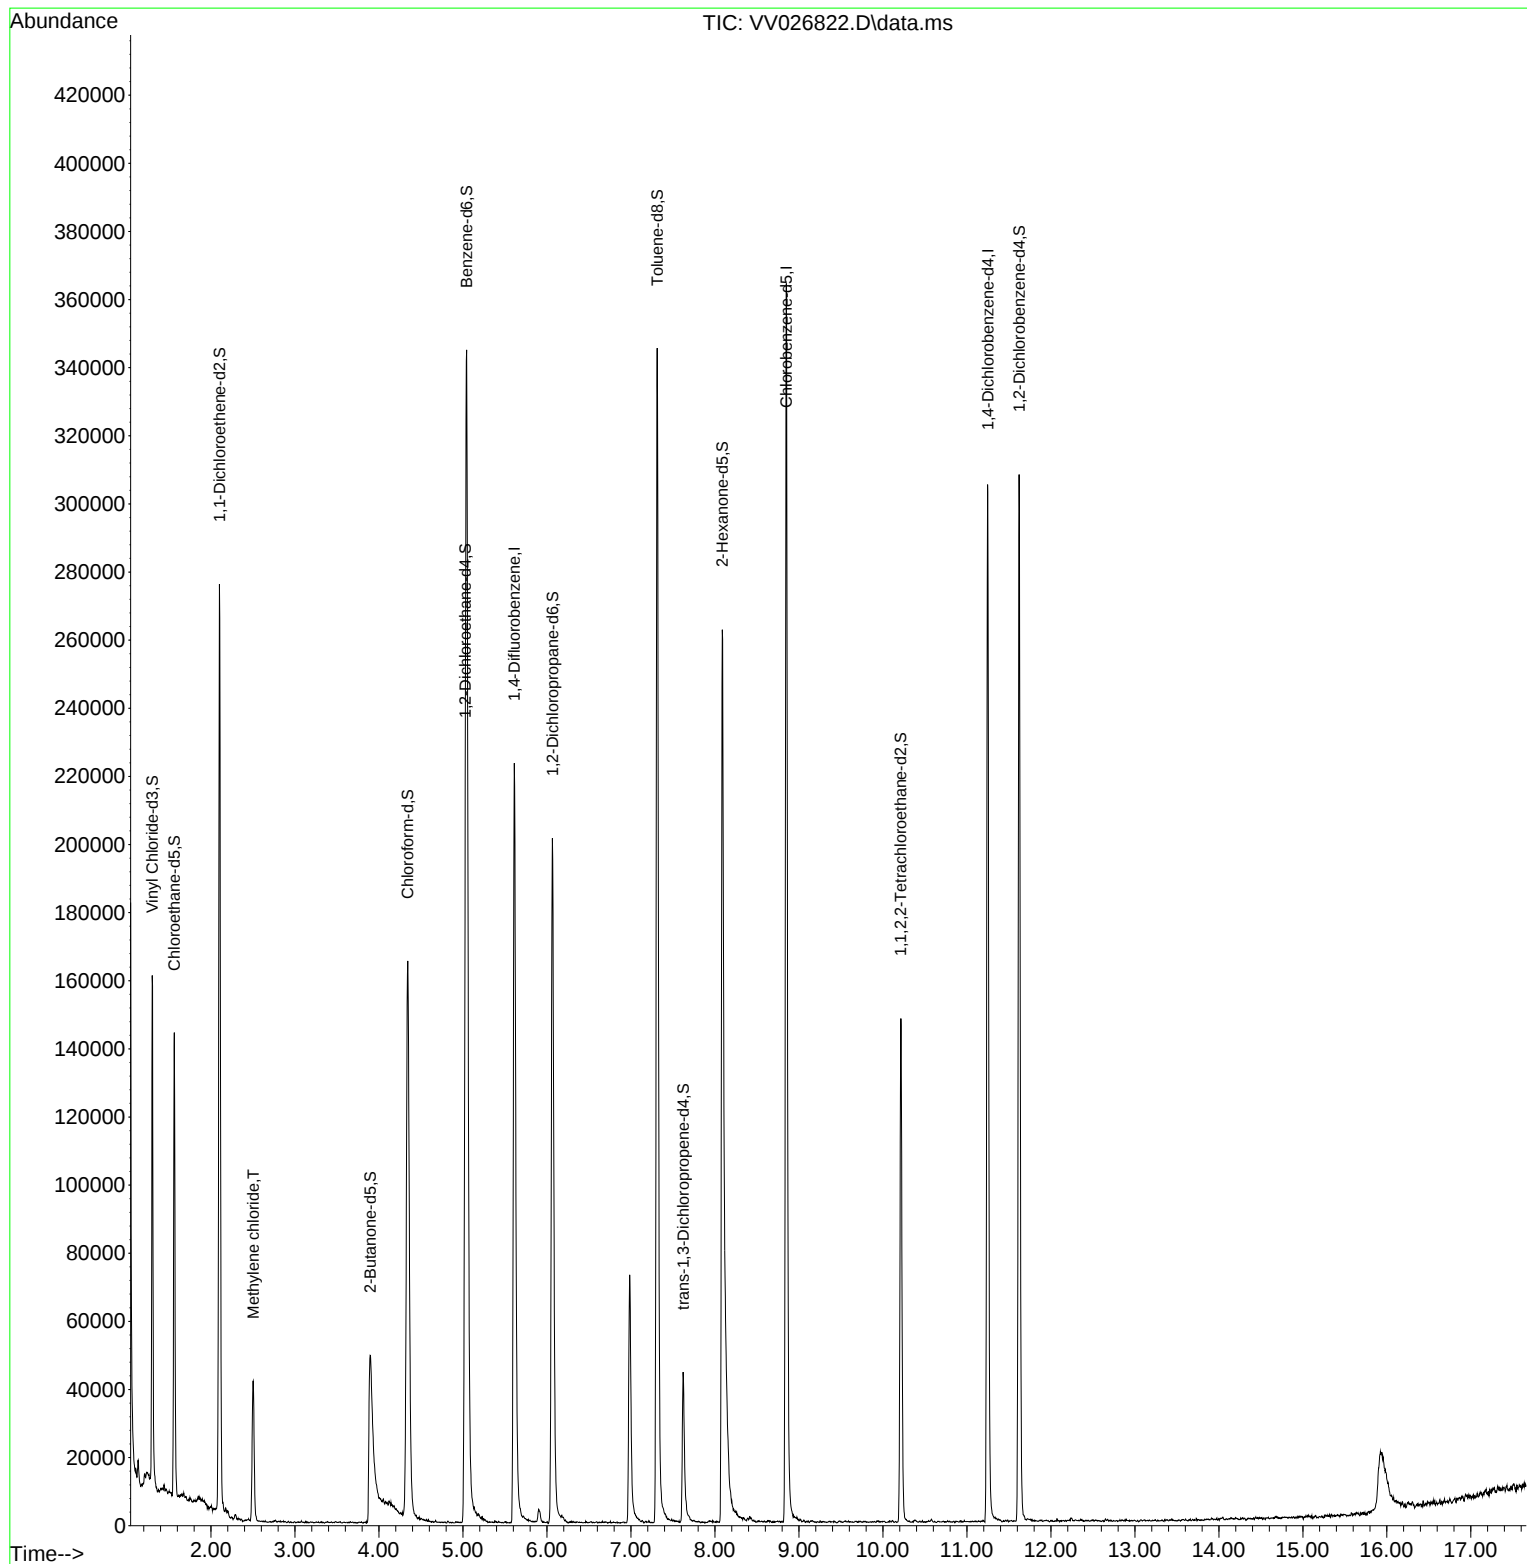

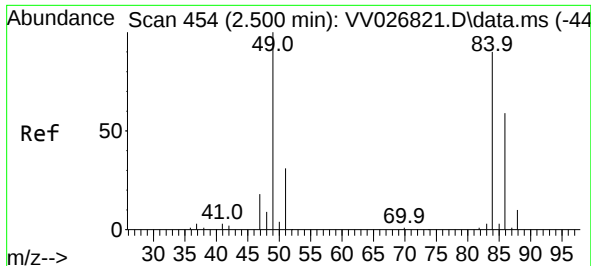

#16
Methylene chloride
Concen: 0.891 ug/L
RT: 2.503 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV026822.D
Acq: 19 Jul 2022 12:38

Instrument :
MSVOA_V
ClientSampleId :
VBLK397

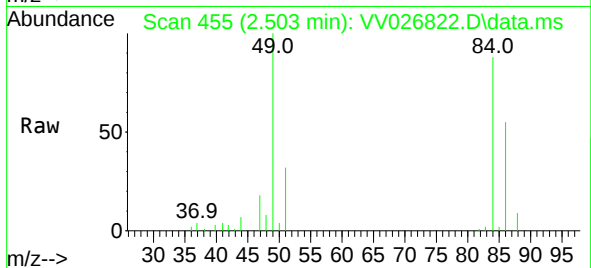

Tgt Ion: 84 Resp: 18465
Ion Ratio Lower Upper
84 100
86 62.6 44.8 83.2
49 113.2 78.7 146.1

