

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
 Data File : VV026823.D
 Acq On : 19 Jul 2022 13:01
 Operator : SY/MD
 Sample : N3709-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Quant Time: Jul 20 05:49:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 20 05:46:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.593	114	260768	5.000	ug/L	-0.02
28) Chlorobenzene-d5	8.863	117	219554	5.000	ug/L	0.01
58) 1,4-Dichlorobenzene-d4	11.249	152	83350	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.294	65	110023	4.625	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.400%
7) Chloroethane-d5	1.555	69	94736	4.609	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	2.095	63	158367	3.468	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.400%
20) 2-Butanone-d5	3.957	46	233849	62.983	ug/L	0.07
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.960%
24) Chloroform-d	4.352	84	203184	4.884	ug/L	0.01
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
26) 1,2-Dichloroethane-d4	5.031	65	99890	5.497	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.000%
32) Benzene-d6	5.037	84	394339	5.911	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	118.200%
36) 1,2-Dichloropropane-d6	6.056	67	126766	6.337	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	126.800%
41) Toluene-d8	7.336	98	272732	4.605	ug/L	0.03
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	7.645	79	31173	4.763	ug/L	0.03
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.200%
46) 2-Hexanone-d5	8.120	63	126179	44.532	ug/L	0.03
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.060%
56) 1,1,2,2-Tetrachloroeth...	10.223	84	79802	5.121	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	84063	5.789	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.800%
Target Compounds						Qvalue
16) Methylene chloride	2.497	84	19582	0.719	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026823.D
Acq On : 19 Jul 2022 13:01
Operator : SY/MD
Sample : N3709-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Time: Jul 20 05:49:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 20 05:46:20 2022
Response via : Initial Calibration

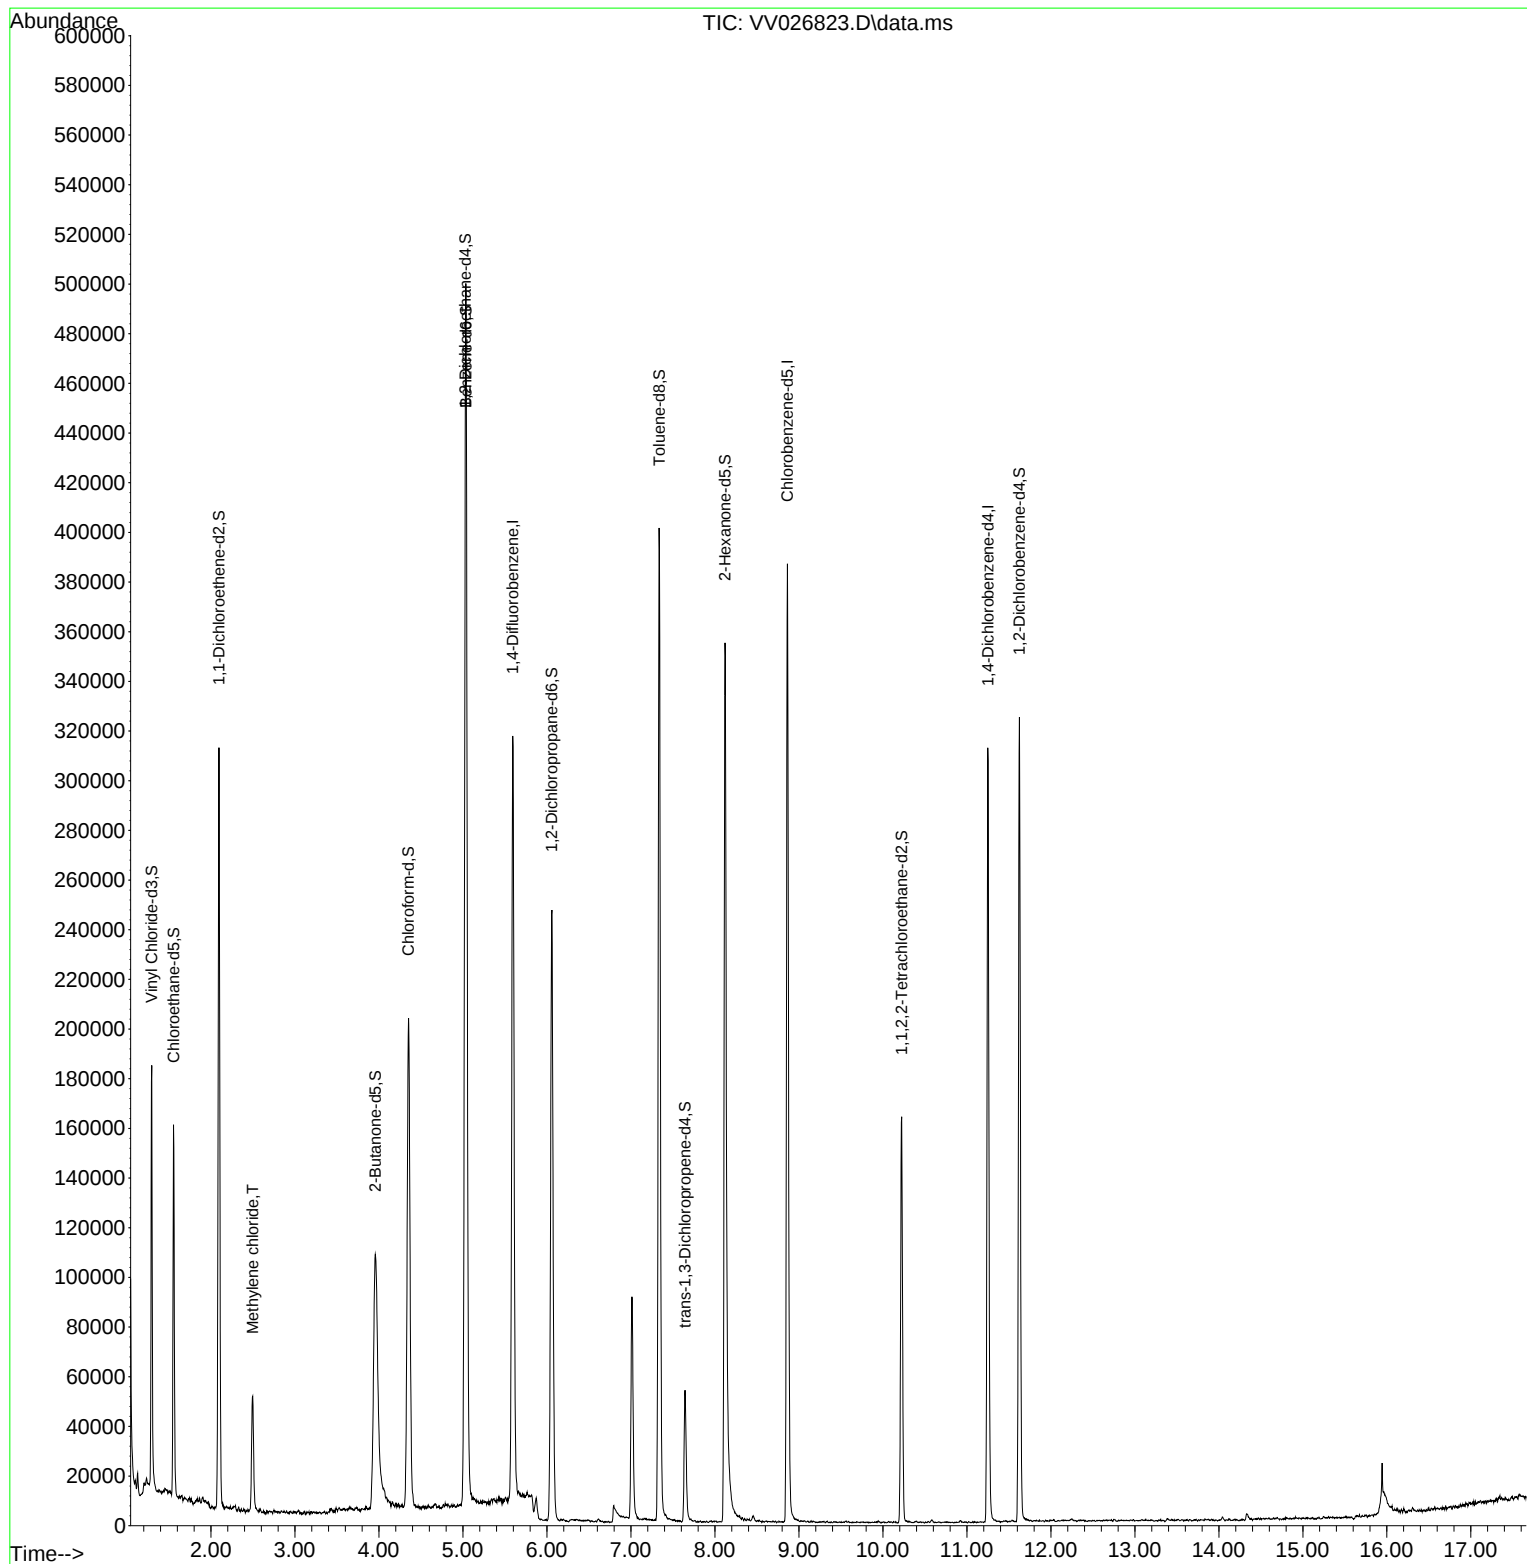

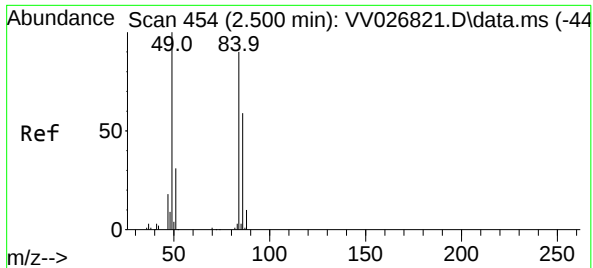

#16
Methylene chloride
Concen: 0.719 ug/L
RT: 2.497 min Scan# 41
Delta R.T. -0.003 min
Lab File: VV026823.D
Acq: 19 Jul 2022 13:01

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Tgt Ion: 84 Resp: 19582
Ion Ratio Lower Upper
84 100
86 67.8 44.8 83.2
49 117.8 78.7 146.1

