

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW071922\
 Data File : VW026825.D
 Acq On : 19 Jul 2022 14:16
 Operator : SY/MD
 Sample : N3710-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jul 20 05:49:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jul 20 05:46:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	213642	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	222781	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	87727	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	98497	5.054	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.000%
7) Chloroethane-d5	1.565	69	86048	5.110	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.200%
11) 1,1-Dichloroethene-d2	2.101	63	141089	3.771	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.400%
20) 2-Butanone-d5	3.896	46	109807	36.098	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	72.200%
24) Chloroform-d	4.346	84	175620	5.153	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
26) 1,2-Dichloroethane-d4	5.031	65	78371	5.264	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.200%
32) Benzene-d6	5.047	84	325754	4.812	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
36) 1,2-Dichloropropane-d6	6.066	67	105906	5.218	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.400%
41) Toluene-d8	7.313	98	239383	3.984	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.600%
43) trans-1,3-Dichloroprop...	7.622	79	27627	4.160	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.200%
46) 2-Hexanone-d5	8.088	63	113165	39.360	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.720%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	72871	4.609	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	79837	5.223	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.400%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	7715	0.346	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026825.D
Acq On : 19 Jul 2022 14:16
Operator : SY/MD
Sample : N3710-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jul 20 05:49:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jul 20 05:46:20 2022
Response via : Initial Calibration

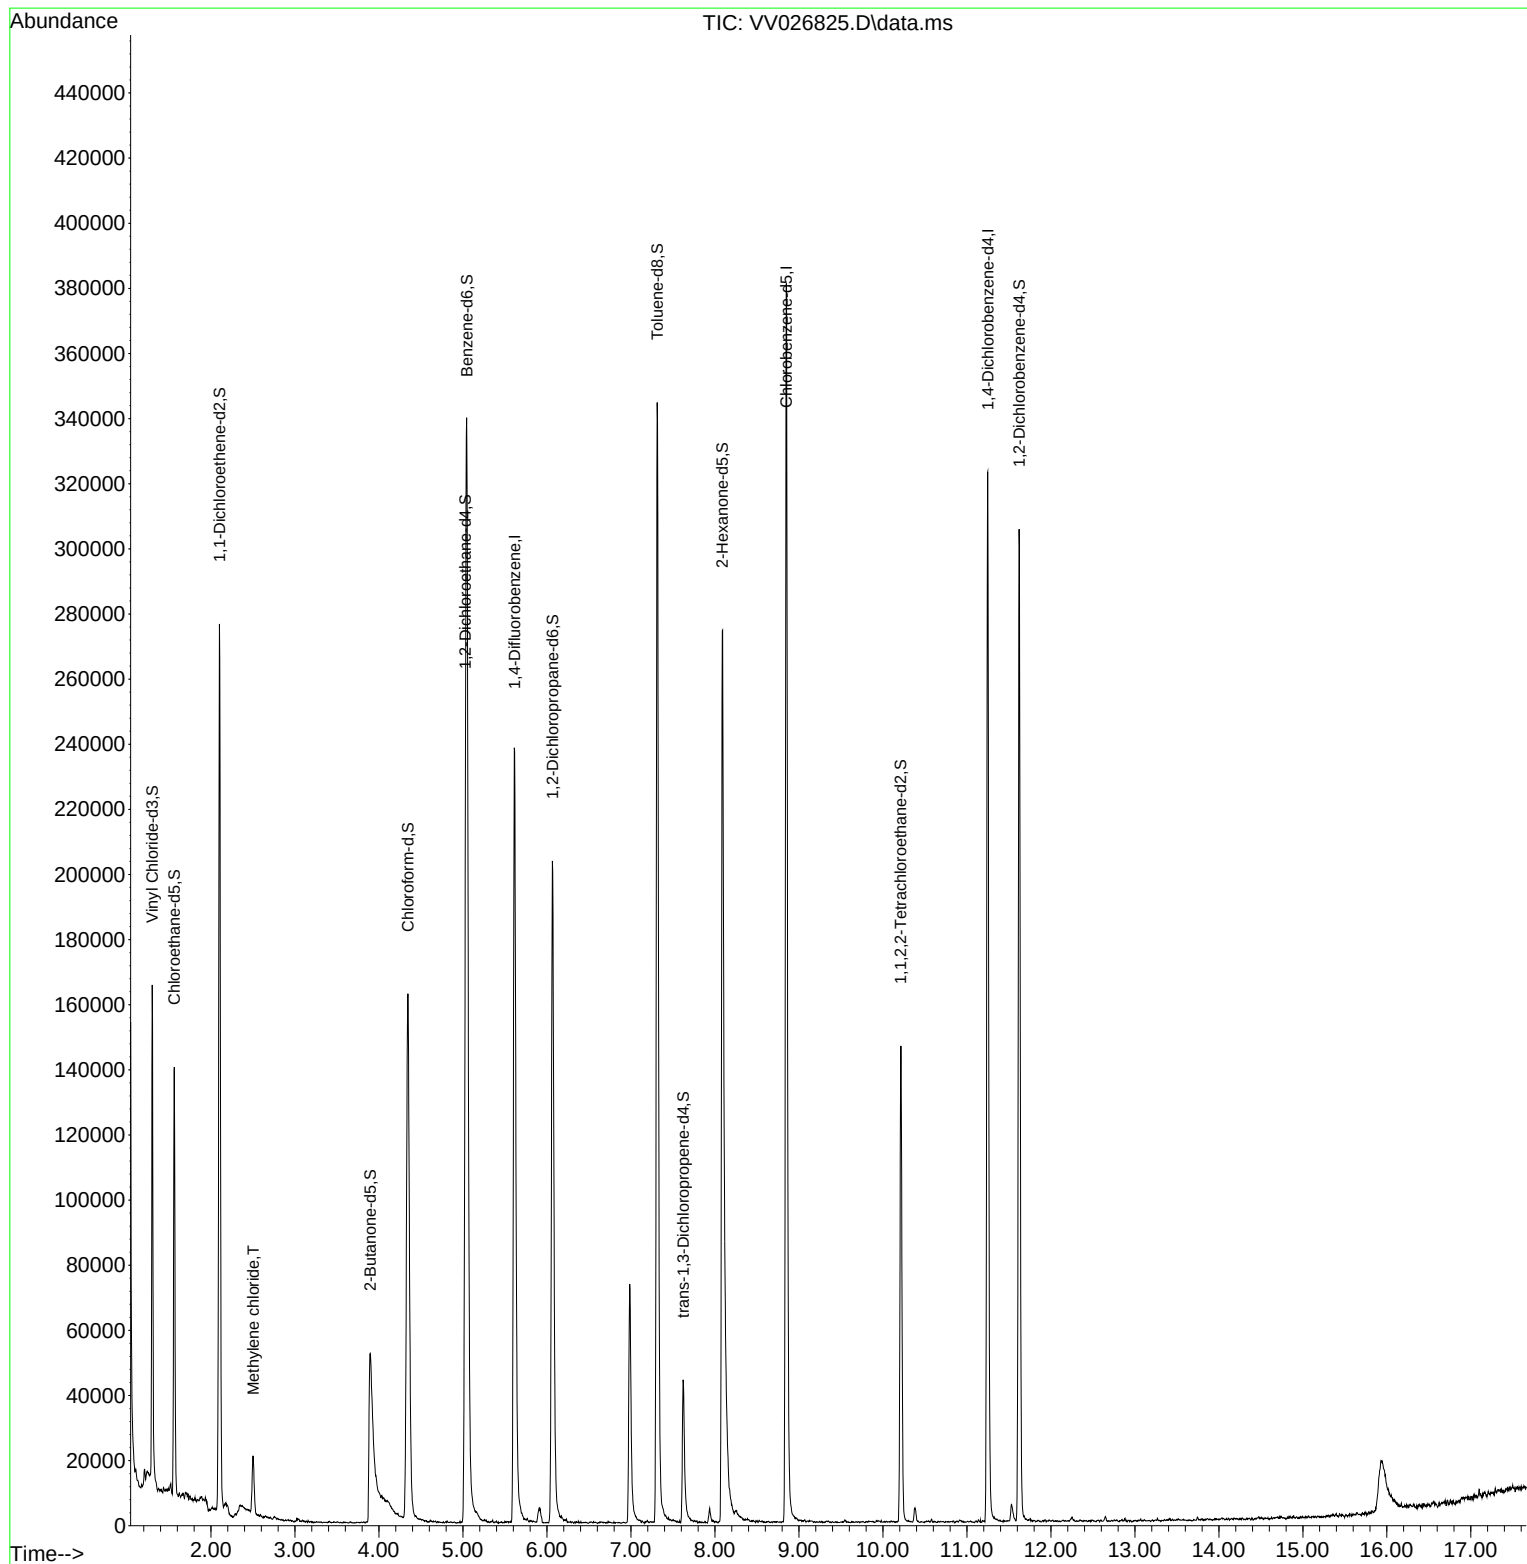

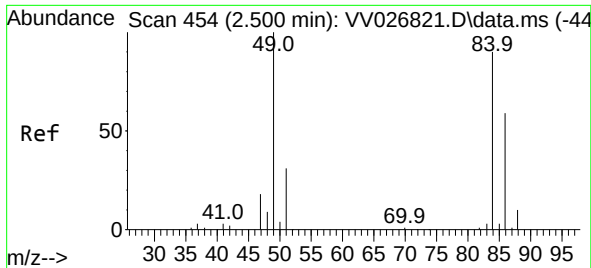

#16
Methylene chloride
Concen: 0.346 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV026825.D
Acq: 19 Jul 2022 14:16

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

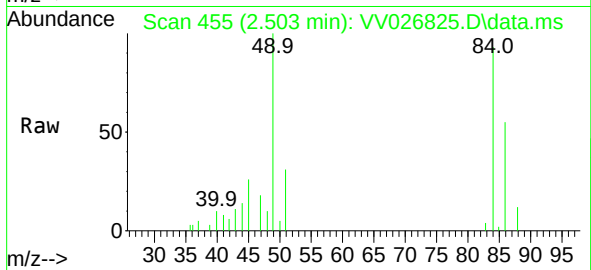

Tgt Ion: 84 Resp: 7715

Ion	Ratio	Lower	Upper
84	100		
86	59.8	44.8	83.2
49	107.9	78.7	146.1

