

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
 Data File : VV026823.D
 Acq On : 19 Jul 2022 13:01
 Operator : SY/MD
 Sample : N3709-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026823.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.294	72	79	98	rVB	171595	180209	17.28%	2.425%
2	1.555	153	160	174	rVB	149858	167382	16.05%	2.252%
3	2.095	318	328	340	rBV	305561	425272	40.77%	5.723%
4	2.497	443	453	465	rBV	45461	74106	7.10%	0.997%
5	3.957	888	907	936	rBV2	102533	383528	36.77%	5.161%
6	4.352	1015	1030	1051	rVB	196260	463173	44.40%	6.233%
7	5.034	1227	1242	1265	rBV2	490773	1043084	100.00%	14.037%
8	5.593	1403	1416	1435	rBV	306692	600504	57.57%	8.081%
9	5.873	1495	1503	1518	rVB7	8836	17505	1.68%	0.236%
10	6.059	1543	1561	1584	rBV	245992	504598	48.38%	6.790%
11	6.796	1781	1790	1801	rBV2	6688	15190	1.46%	0.204%
12	7.011	1846	1857	1877	rBV	89154	157727	15.12%	2.122%
13	7.336	1946	1958	1980	rBV	399656	699020	67.01%	9.407%
14	7.645	2041	2054	2072	rBV	53179	94847	9.09%	1.276%
15	8.120	2187	2202	2246	rBV	354102	710839	68.15%	9.566%
16	8.863	2422	2433	2460	rBV	385617	620747	59.51%	8.353%
17	10.223	2844	2856	2870	rBV	163455	257613	24.70%	3.467%
18	11.249	3165	3175	3198	rBV	311735	482723	46.28%	6.496%
19	11.625	3280	3292	3310	rBV	324041	509378	48.83%	6.855%
20	15.943	4622	4635	4639	rBV	19564	23763	2.28%	0.320%




Sum of corrected areas: 7431208

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026823.D
Acq On : 19 Jul 2022 13:01
Operator : SY/MD
Sample : N3709-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

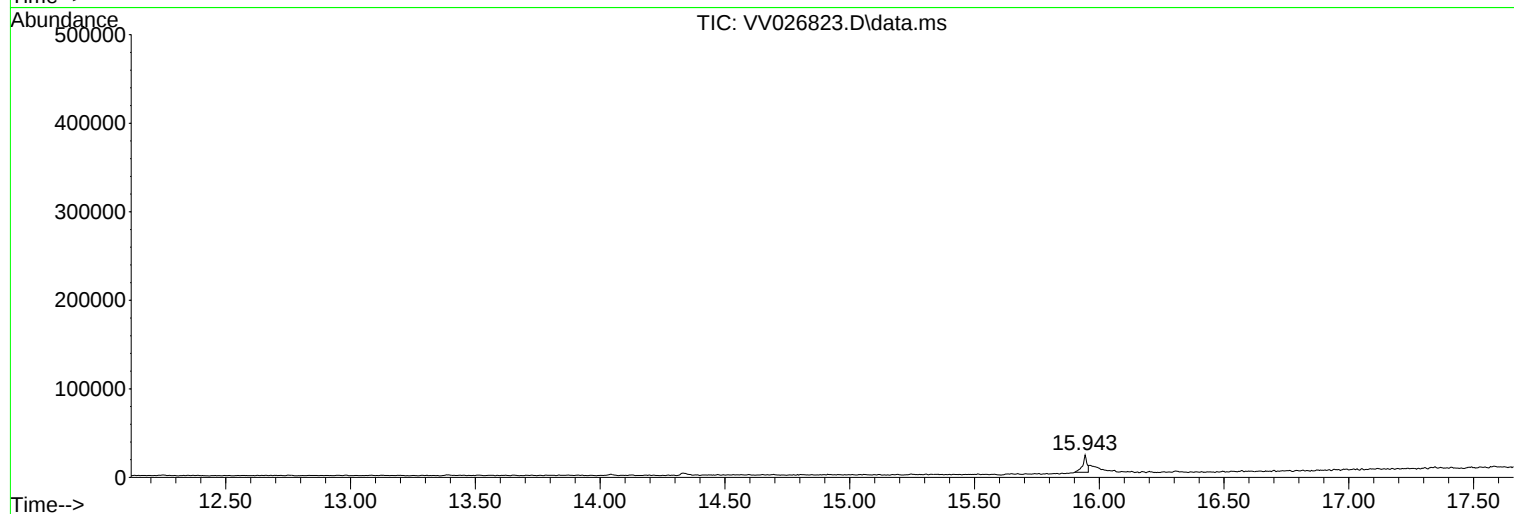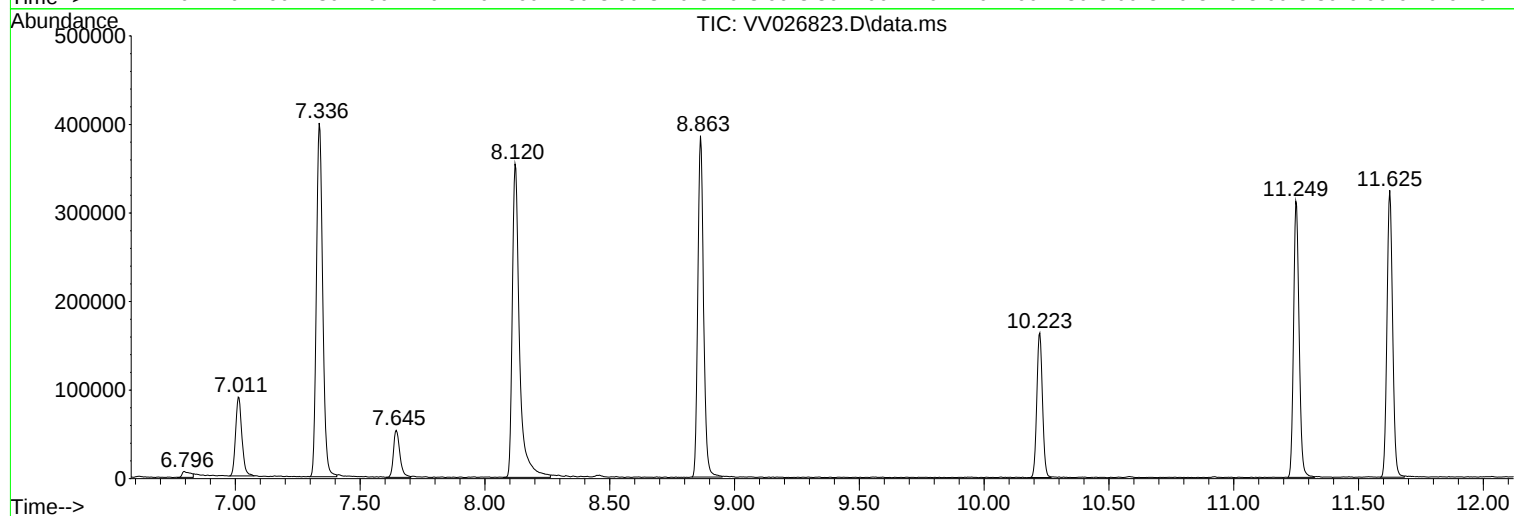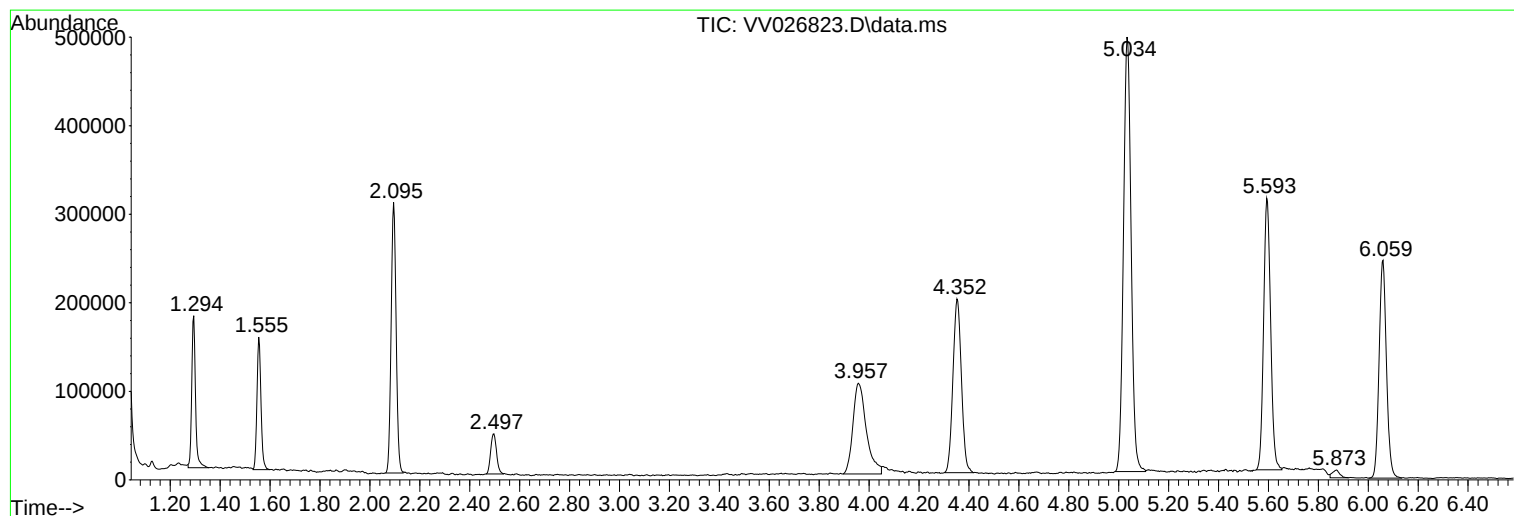

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026823.D
Acq On : 19 Jul 2022 13:01
Operator : SY/MD
Sample : N3709-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026823.D
Acq On : 19 Jul 2022 13:01
Operator : SY/MD
Sample : N3709-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc