

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
 Data File : VV026824.D
 Acq On : 19 Jul 2022 13:51
 Operator : SY/MD
 Sample : N3704-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.230	54	59	69	rBV2	9400	14725	1.55%	0.216%
2	1.294	72	79	98	rVB	157012	165864	17.42%	2.435%
3	1.558	153	161	174	rVB	134011	157568	16.55%	2.314%
4	2.111	323	333	355	rVB	279174	396774	41.66%	5.826%
5	2.510	446	457	466	rBV	24453	40021	4.20%	0.588%
6	3.957	886	907	936	rBV	73967	318610	33.46%	4.678%
7	4.349	1014	1029	1047	rVB2	172560	412835	43.35%	6.062%
8	5.037	1228	1243	1268	rBV2	441024	952308	100.00%	13.983%
9	5.613	1406	1422	1446	rVB	321836	643006	67.52%	9.442%
10	5.896	1499	1510	1520	rVB6	5753	10764	1.13%	0.158%
11	6.076	1550	1566	1590	rBV	214584	439169	46.12%	6.449%
12	6.735	1760	1771	1781	rBV2	7689	17566	1.84%	0.258%
13	6.998	1841	1853	1874	rBV	77113	140911	14.80%	2.069%
14	7.323	1942	1954	1975	rBV	348206	605452	63.58%	8.890%
15	7.635	2039	2051	2071	rBV	45609	80480	8.45%	1.182%
16	8.114	2185	2200	2231	rBV	297942	592616	62.23%	8.702%
17	8.857	2420	2431	2454	rBV	388702	628115	65.96%	9.223%
18	10.220	2843	2855	2869	rBV	144597	225496	23.68%	3.311%
19	11.249	3162	3175	3194	rBV	325296	499881	52.49%	7.340%
20	11.622	3280	3291	3305	rBV	289182	445508	46.78%	6.542%
21	15.937	4617	4633	4635	rBV	10120	22619	2.38%	0.332%




Sum of corrected areas: 6810288

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026824.D
Acq On : 19 Jul 2022 13:51
Operator : SY/MD
Sample : N3704-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

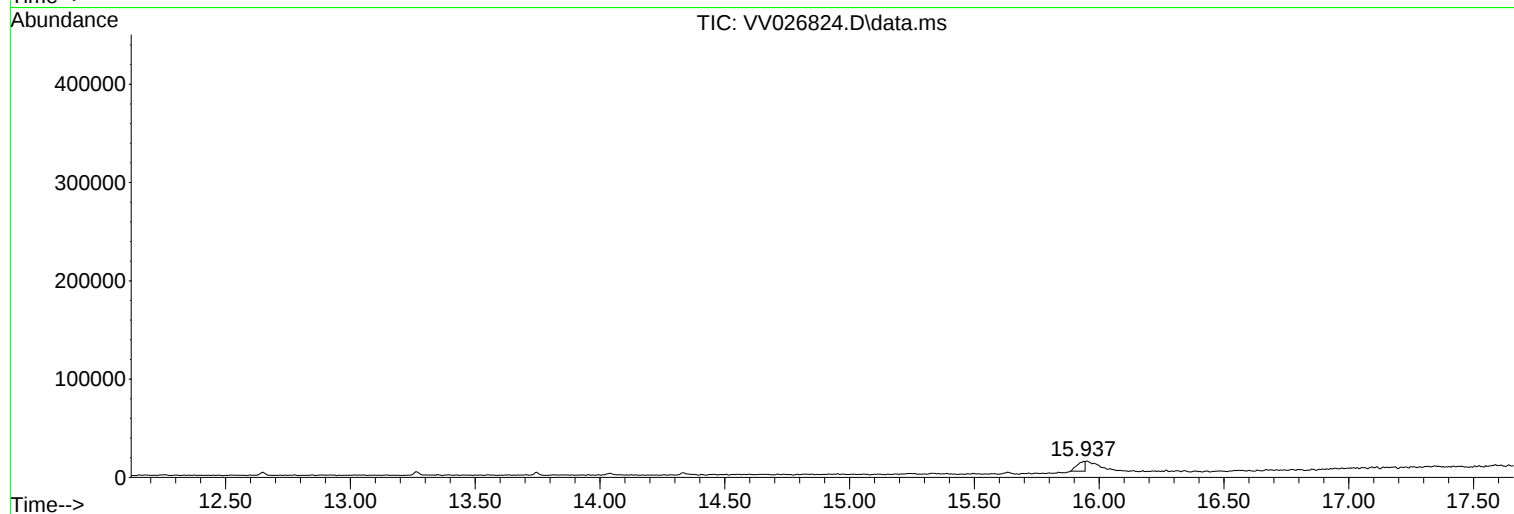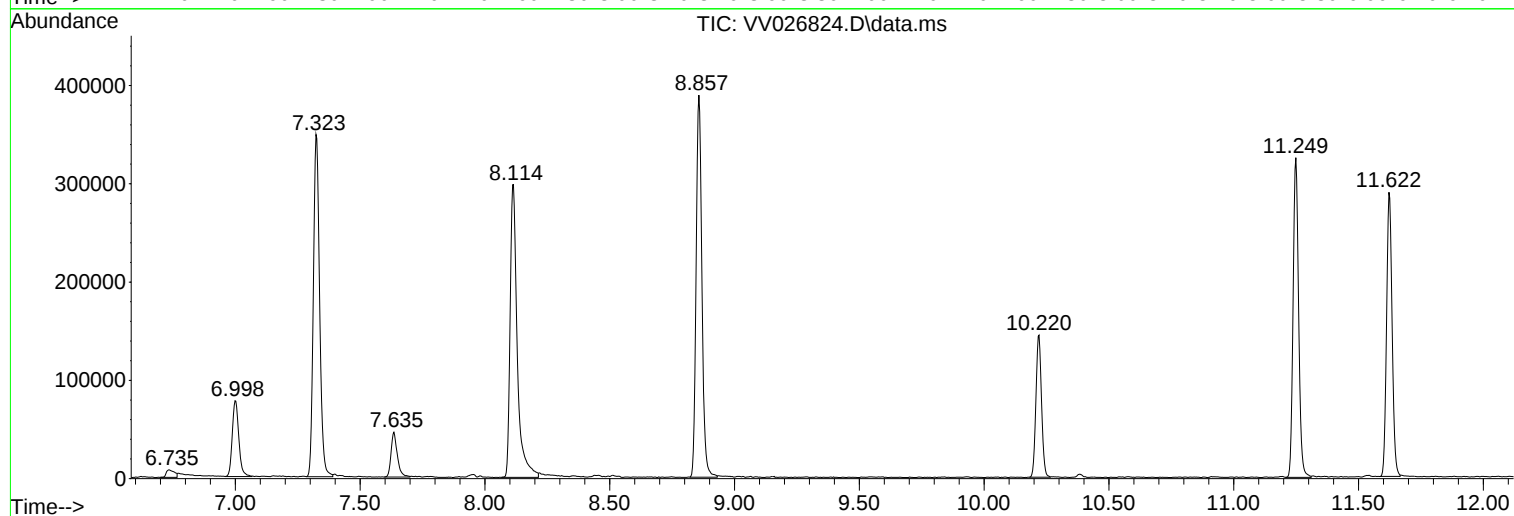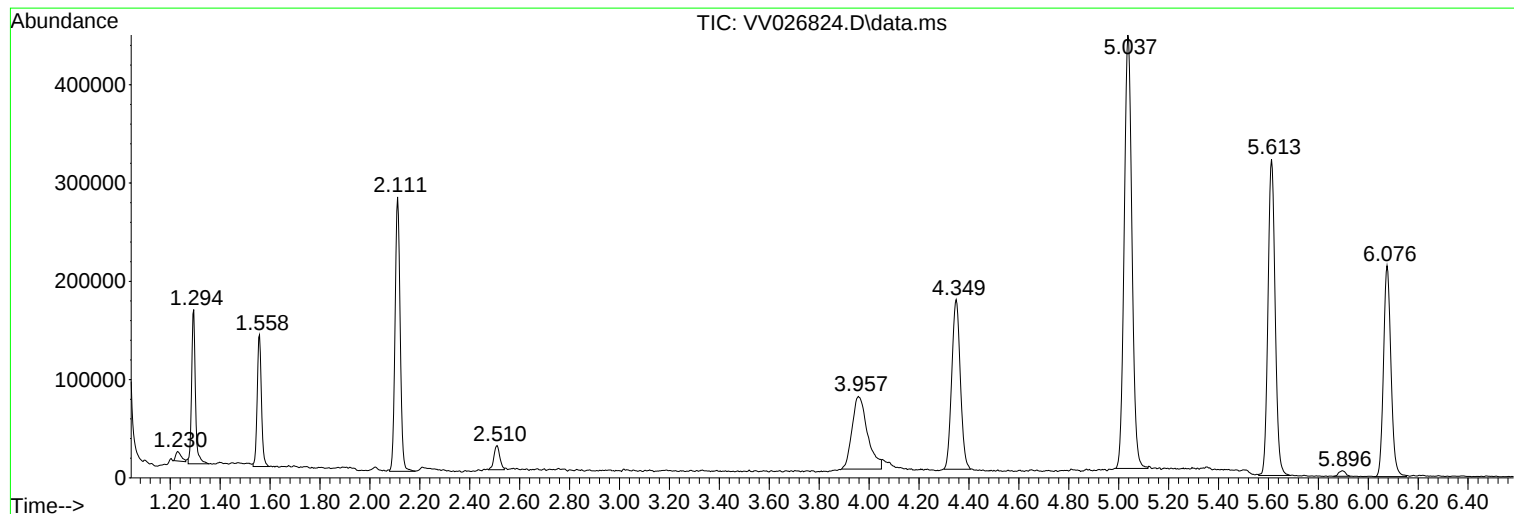

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026824.D
Acq On : 19 Jul 2022 13:51
Operator : SY/MD
Sample : N3704-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026824.D
Acq On : 19 Jul 2022 13:51
Operator : SY/MD
Sample : N3704-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc