

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
 Data File : VV026825.D
 Acq On : 19 Jul 2022 14:16
 Operator : SY/MD
 Sample : N3710-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	101	rVB	155435	166523	19.39%	2.575%
2	1.565	155	163	178	rVB	131934	153304	17.85%	2.370%
3	2.101	319	330	345	rBV	271819	386887	45.04%	5.982%
4	2.500	445	454	466	rVB2	17988	30702	3.57%	0.475%
5	3.896	878	888	908	rBV2	51710	170742	19.88%	2.640%
6	4.346	1012	1028	1054	rBV	160748	398007	46.33%	6.154%
7	5.043	1227	1245	1280	rBV2	339255	859024	100.00%	13.282%
8	5.613	1409	1422	1448	rBV	237933	493477	57.45%	7.630%
9	5.908	1504	1514	1527	rVB7	4649	10671	1.24%	0.165%
10	6.066	1549	1563	1590	rBV	203276	423252	49.27%	6.544%
11	6.986	1834	1849	1873	rBV	73409	141991	16.53%	2.196%
12	7.313	1940	1951	1980	rBV	343842	610040	71.02%	9.433%
13	7.622	2038	2047	2071	rBV2	43958	84643	9.85%	1.309%
14	8.092	2182	2193	2236	rBV	273775	630500	73.40%	9.749%
15	8.850	2417	2429	2457	rBV	380386	639432	74.44%	9.887%
16	10.214	2843	2853	2870	rBV	145996	233095	27.13%	3.604%
17	11.249	3164	3175	3198	rBV	322430	507195	59.04%	7.842%
18	11.532	3255	3263	3278	rBV5	5074	9398	1.09%	0.145%
19	11.622	3279	3291	3308	rBV	304574	478128	55.66%	7.393%
20	15.930	4609	4631	4634	rBV	15489	40352	4.70%	0.624%




Sum of corrected areas: 6467363

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026825.D
Acq On : 19 Jul 2022 14:16
Operator : SY/MD
Sample : N3710-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

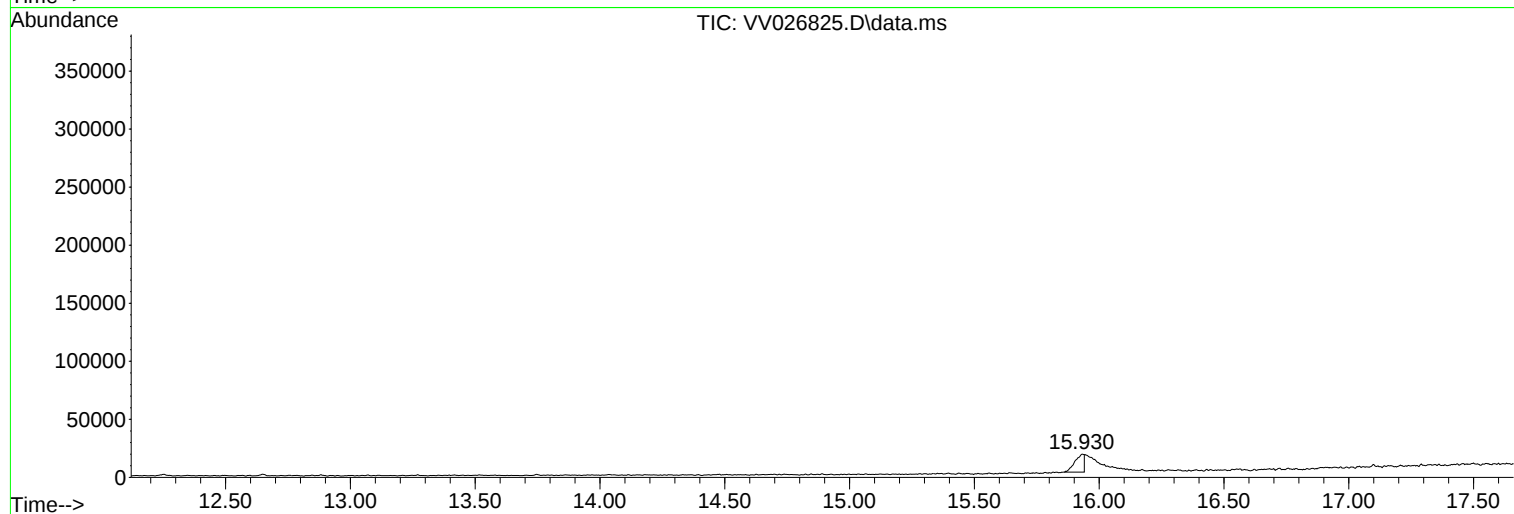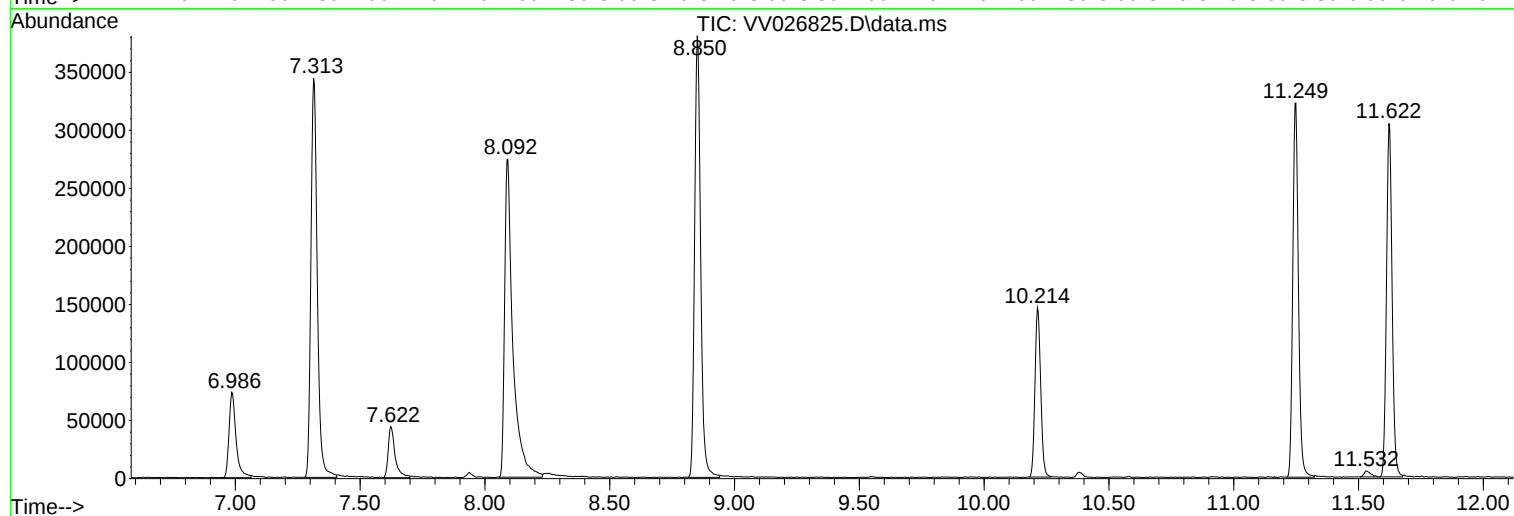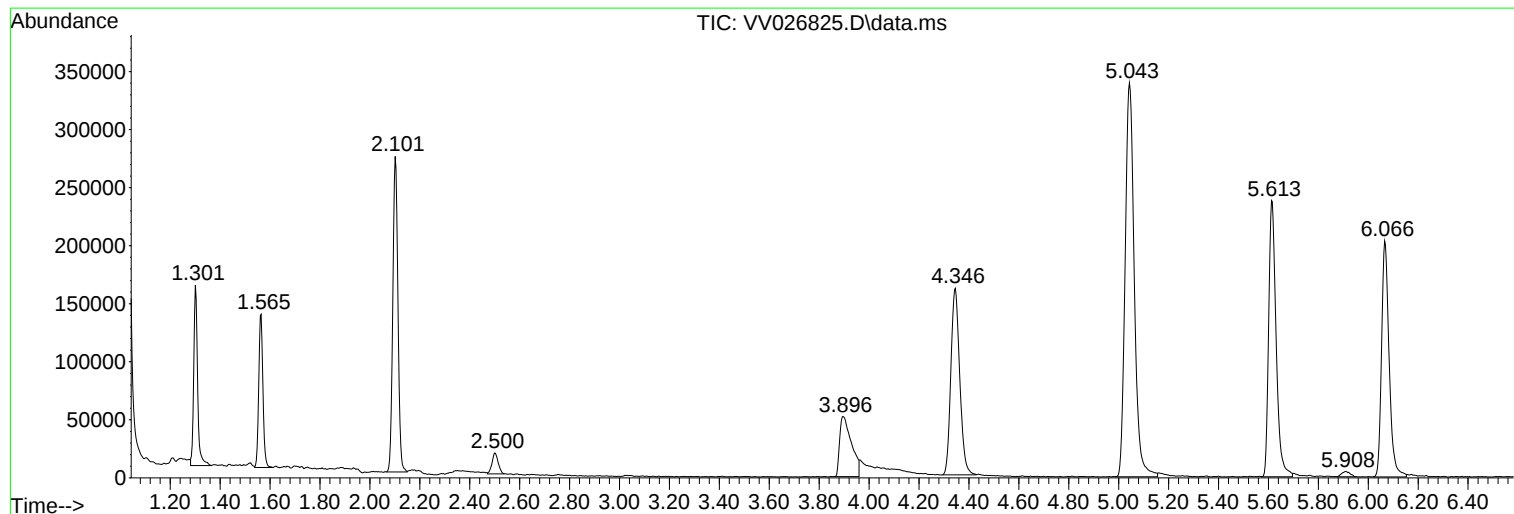

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026825.D
Acq On : 19 Jul 2022 14:16
Operator : SY/MD
Sample : N3710-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026825.D
Acq On : 19 Jul 2022 14:16
Operator : SY/MD
Sample : N3710-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc