

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
 Data File : VV026827.D
 Acq On : 19 Jul 2022 15:29
 Operator : SY/MD
 Sample : N3754-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBHQ6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026827.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	45	rVB	159711	158063	10.25%	0.855%
2	1.304	75	82	102	rVB2	261844	289147	18.75%	1.564%
3	1.581	156	168	188	rVB2	398723	567555	36.80%	3.070%
4	2.111	320	333	346	rBV3	881720	1504857	97.56%	8.139%
5	2.191	346	358	425	rVV	122693	585596	37.96%	3.167%
6	2.439	425	435	446	rVV	42366	89285	5.79%	0.483%
7	2.500	446	454	472	rVB	69514	121125	7.85%	0.655%
8	2.757	518	534	552	rBV	143977	252755	16.39%	1.367%
9	3.185	648	667	686	rBV	76922	162417	10.53%	0.878%
10	3.908	878	892	941	rBV2	201077	667776	43.29%	3.612%
11	4.246	982	997	1014	rBV2	125271	311401	20.19%	1.684%
12	4.368	1015	1035	1063	rVB3	348118	1122345	72.76%	6.070%
13	4.603	1091	1108	1129	rBV4	79051	200668	13.01%	1.085%
14	4.825	1161	1177	1197	rBV2	112484	272356	17.66%	1.473%
15	5.043	1226	1245	1264	rBV3	298804	754778	48.93%	4.082%
16	5.133	1265	1273	1295	rVB2	42470	100074	6.49%	0.541%
17	5.616	1408	1423	1453	rBV2	242821	508049	32.94%	2.748%
18	5.915	1503	1516	1536	rBV	119476	250007	16.21%	1.352%
19	6.069	1550	1564	1595	rBV2	190341	398869	25.86%	2.157%
20	6.989	1839	1850	1855	rBV2	73599	122940	7.97%	0.665%
21	7.027	1855	1862	1886	rVB	164609	311398	20.19%	1.684%
22	7.230	1906	1925	1942	rBV	802058	1542464	100.00%	8.343%
23	7.313	1942	1951	1972	rVB	373399	682054	44.22%	3.689%
24	7.625	2036	2048	2051	rBV	52969	75509	4.90%	0.408%
25	7.654	2053	2057	2080	rVB	72378	121653	7.89%	0.658%
26	7.841	2103	2115	2137	rBV	88453	157609	10.22%	0.852%
27	7.976	2139	2157	2173	rBV	217669	372510	24.15%	2.015%
28	8.091	2182	2193	2233	rBV	410207	821028	53.23%	4.441%
29	8.352	2263	2274	2299	rBV	99055	170742	11.07%	0.923%
30	8.854	2415	2430	2433	rBV	426969	619427	40.16%	3.350%
31	8.879	2434	2438	2471	rVB	584285	886975	57.50%	4.797%
32	9.731	2692	2703	2721	rBV	48088	81989	5.32%	0.443%
33	10.217	2839	2854	2881	rBV2	167430	348551	22.60%	1.885%
34	10.915	3059	3071	3088	rBV	421393	641377	41.58%	3.469%
35	11.181	3142	3154	3165	rBV	265886	418620	27.14%	2.264%
36	11.249	3165	3175	3198	rVB2	431392	913151	59.20%	4.939%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026827.D
Acq On : 19 Jul 2022 15:29
Operator : SY/MD
Sample : N3754-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBHQ6

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Title : TRACE VOA SFAM1.0

37	11.625	3280	3292	3312	rBV	335286	539267	34.96%	2.917%
38	12.644	3597	3609	3628	rBV	406448	626648	40.63%	3.389%
39	13.258	3788	3800	3819	rBV	296023	463690	30.06%	2.508%
40	13.741	3938	3950	3966	rBV	162802	254216	16.48%	1.375%




Sum of corrected areas: 18488941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026827.D
Acq On : 19 Jul 2022 15:29
Operator : SY/MD
Sample : N3754-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBHQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

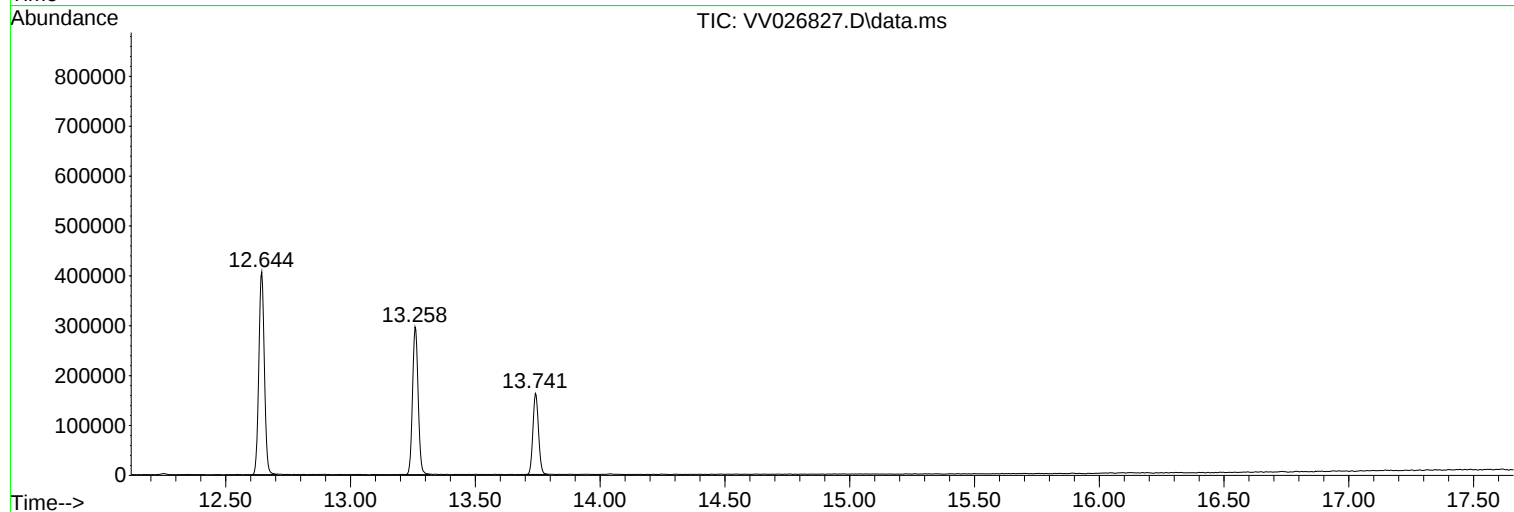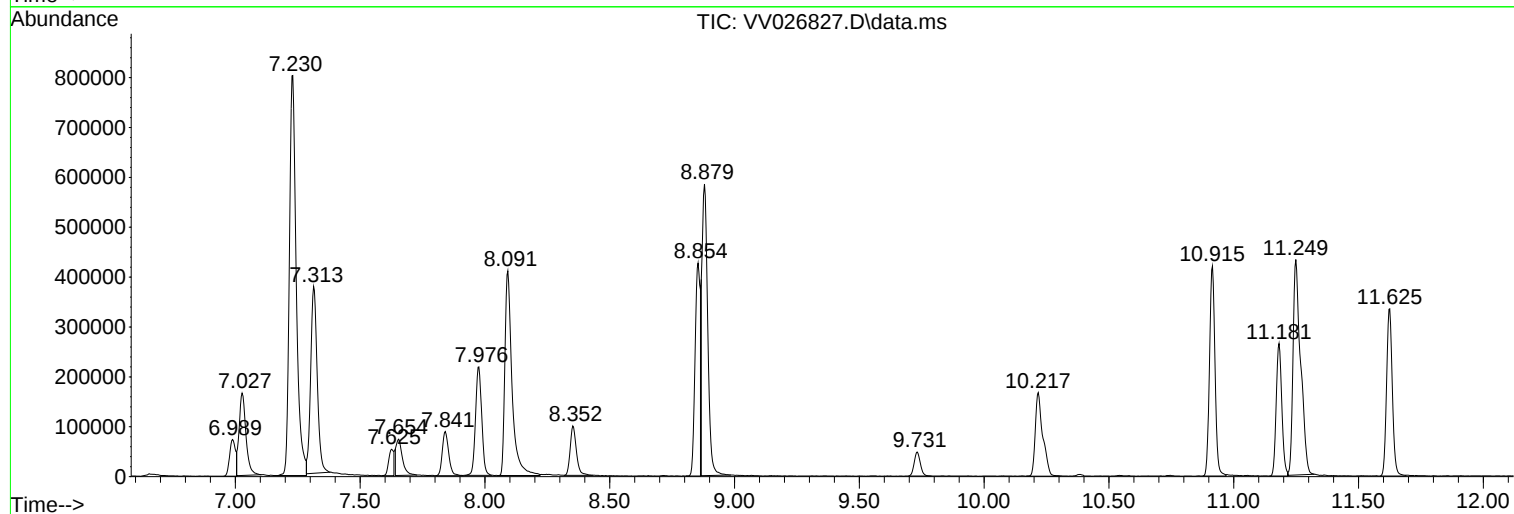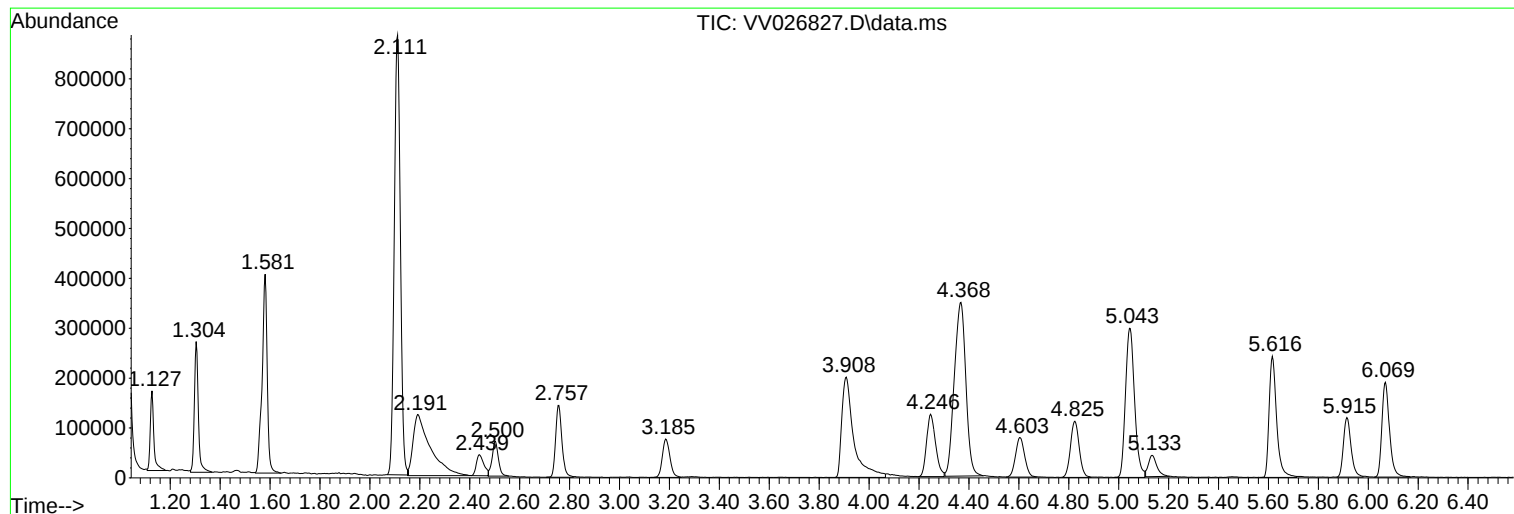

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026827.D
Acq On : 19 Jul 2022 15:29
Operator : SY/MD
Sample : N3754-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBHQ6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzene, 1,3,5-trichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.644	3.43 ug/L	626648	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
2			Benzene, 1,2,4-trichloro-	180	C6H3Cl3	000120-82-1	98
3			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98
4			Benzene, 1,3,5-trichloro-	180	C6H3Cl3	000108-70-3	98
5			Benzene, 1,2,3-trichloro-	180	C6H3Cl3	000087-61-6	98

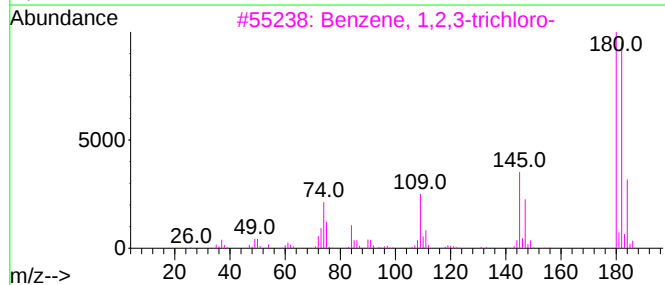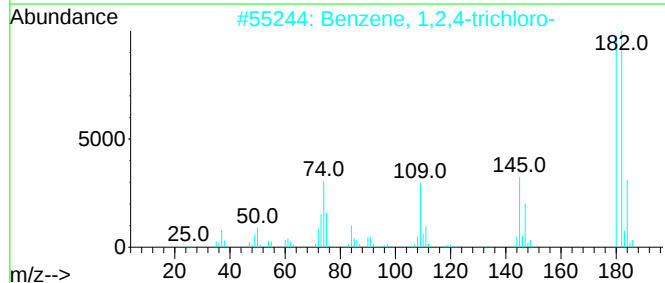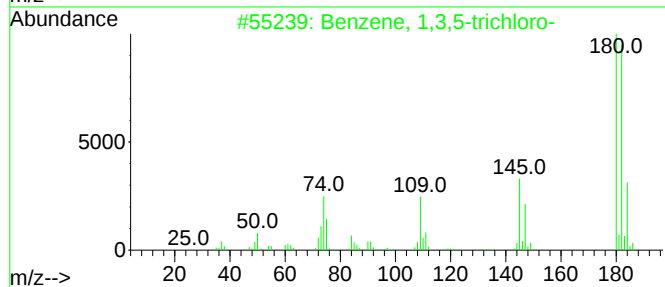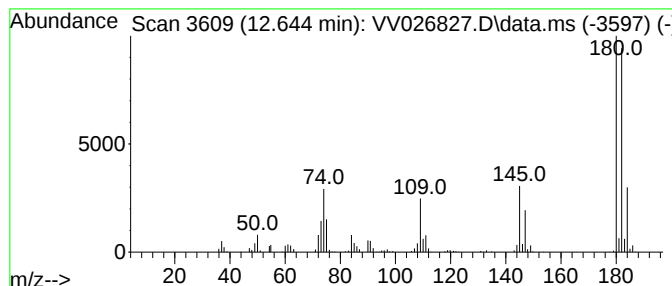

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
Data File : VV026827.D
Acq On : 19 Jul 2022 15:29
Operator : SY/MD
Sample : N3754-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBHQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzene, 1,3,5-...	12.644	3.4	ug/L	626648	3	11.249	913151	5.0