
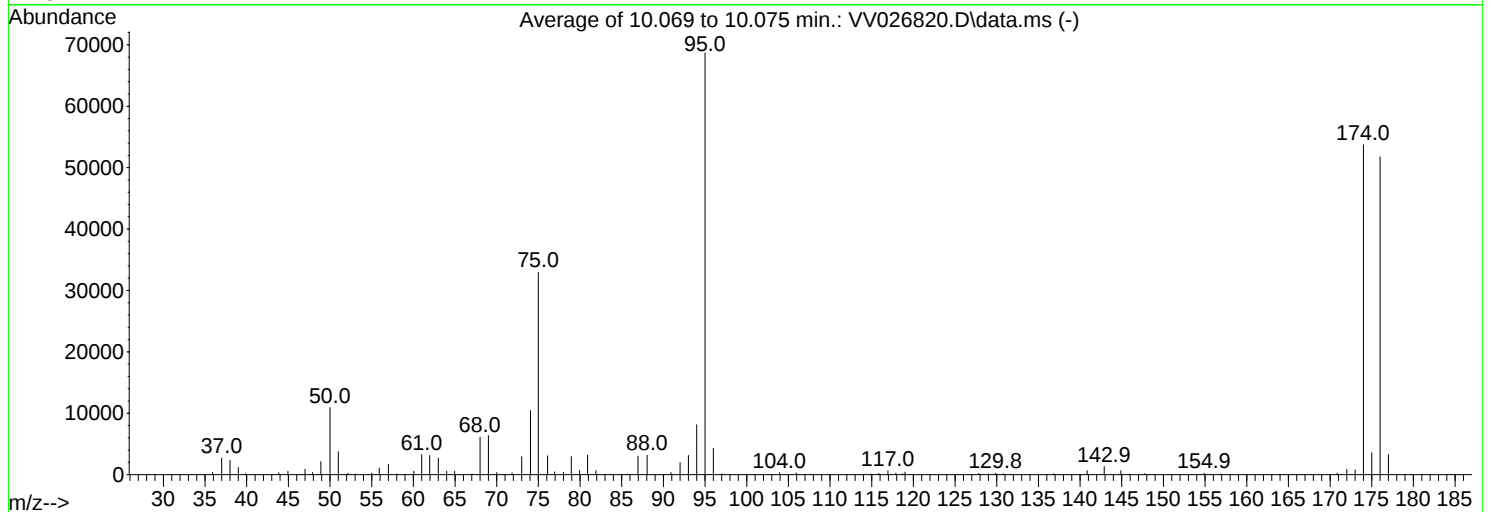


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071922\
 Data File : VV026820.D
 Acq On : 19 Jul 2022 09:11
 Operator : SY/MD
 Sample : BFB348
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB348

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Jul 21 01:47:16 2022

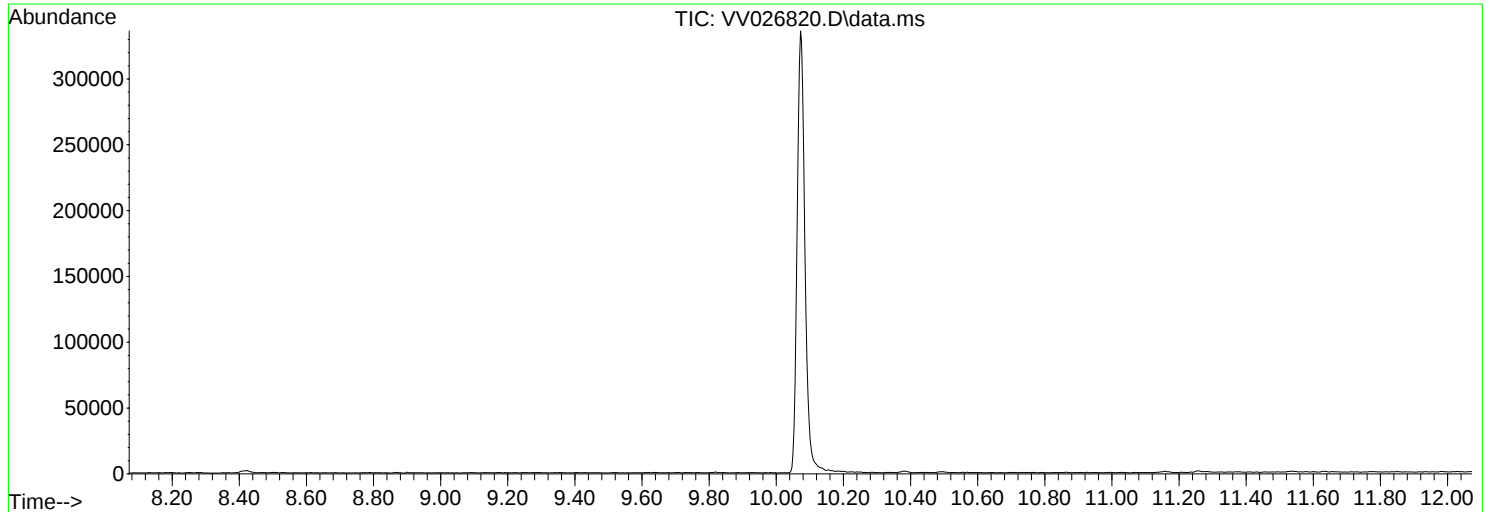

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	10909	PASS
75	95	30	80	48.0	32947	PASS
95	95	100	100	100.0	68701	PASS
96	95	5	9	6.2	4283	PASS
173	174	0.00	2	1.4	778	PASS
174	95	50	120	78.2	53720	PASS
175	174	5	9	6.6	3571	PASS
176	174	95	105	96.3	51749	PASS
177	176	5	10	6.4	3296	PASS

m/z	Abundance
39.90	316.0
43.80	580.0

Instrument :
MSVOA_V
ClientSampleId :
BFB348

m/z	Abundance
35.90	369.0
37.00	2598.0
38.00	2390.0
39.00	1093.0
39.90	430.0
44.00	884.0
44.90	604.0
47.00	792.0
47.90	325.0
48.90	2123.0
50.00	10413.0
51.00	3590.0
52.10	212.0
55.00	289.0
55.90	959.0
57.00	1634.0
58.10	132.0
60.00	540.0
61.00	3236.0
61.90	3041.0
63.00	2644.0
64.00	591.0
64.90	576.0
67.10	198.0
68.00	6078.0
69.00	6168.0
70.10	340.0
71.90	324.0
73.00	2785.0
74.00	10040.0
75.00	32016.0
76.10	2980.0
77.00	452.0
77.90	375.0
79.00	2733.0
80.00	640.0
80.90	3109.0
81.90	577.0
85.70	164.0
86.90	2926.0
88.10	2909.0
90.90	295.0
92.00	1960.0
93.00	3031.0
94.00	7813.0
95.00	66456.0
96.00	4051.0
97.00	137.0
103.90	317.0
105.90	277.0
114.90	109.0
115.90	219.0
116.90	537.0
117.90	309.0
119.00	404.0
127.80	268.0
129.00	158.0
129.90	258.0
130.80	134.0
136.90	113.0
140.90	570.0
142.90	1176.0
144.90	596.0
145.90	134.0
147.70	197.0
154.90	261.0
156.90	117.0
158.90	105.0
170.90	323.0
172.00	794.0
173.00	677.0
174.00	50328.0
175.00	3261.0
176.00	48560.0
177.00	3377.0

Instrument :
MSVOA_V
ClientSampleId :
BFB348

m/z	Abundance
35.90	398.0
37.00	2752.0
38.00	2431.0
39.00	1198.0
39.90	485.0
43.90	924.0
44.90	520.0
47.00	900.0
47.90	345.0
48.90	2127.0
50.00	11297.0
51.00	3822.0
52.10	237.0
53.10	102.0
55.00	269.0
55.90	1103.0
57.00	1699.0
58.00	152.0
60.10	597.0
61.00	3441.0
62.00	3194.0
63.00	2778.0
64.00	595.0
64.90	571.0
67.00	151.0
68.00	6263.0
69.00	6571.0
70.00	340.0
71.80	242.0
73.00	3045.0
74.10	10750.0
75.00	34040.0
76.10	3204.0
76.90	460.0
78.00	407.0
79.00	3018.0
80.00	711.0
80.90	3296.0
81.90	676.0
85.70	123.0
87.00	3164.0
88.00	3274.0
90.90	362.0
92.00	2030.0
93.00	3224.0
94.00	8426.0
95.00	71176.0
96.00	4432.0
97.00	138.0
103.90	363.0
105.90	319.0
114.90	126.0
115.90	218.0
117.00	650.0
117.90	270.0
118.70	403.0
119.00	416.0
127.80	247.0
129.00	176.0
129.90	251.0
130.80	167.0
136.80	162.0
140.80	652.0
142.90	1363.0
144.90	674.0
145.80	135.0
147.80	214.0
154.90	241.0
156.80	121.0
170.80	252.0
172.00	913.0
173.00	813.0
174.00	55528.0
175.00	3634.0
176.00	53312.0
177.00	3367.0

Instrument :
MSVOA_V
ClientSampleId :
BFB348

m/z	Abundance
35.90	361.0
37.00	2681.0
38.00	2220.0
39.00	1147.0
39.80	491.0
43.90	913.0
45.00	513.0
47.00	1005.0
47.90	350.0
48.90	2056.0
50.00	11016.0
51.00	3738.0
52.20	198.0
53.00	133.0
55.00	219.0
55.90	1145.0
57.00	1650.0
58.00	126.0
60.00	575.0
61.00	3107.0
62.00	3154.0
63.00	2674.0
64.00	547.0
65.00	574.0
66.80	159.0
68.00	5901.0
69.00	6384.0
69.90	370.0
71.90	217.0
73.00	2942.0
74.00	10484.0
75.00	32784.0
76.10	3026.0
76.90	431.0
78.10	412.0
78.90	3121.0
79.90	703.0
80.90	3153.0
81.90	696.0
87.00	3011.0
88.00	3286.0
90.90	407.0
92.00	1851.0
93.00	3118.0
94.00	8167.0
95.00	68472.0
96.00	4367.0
97.00	129.0
97.30	141.0
104.00	380.0
106.00	289.0
114.80	108.0
115.80	193.0
116.90	684.0
117.90	218.0
119.00	414.0
128.00	220.0
129.00	149.0
129.70	241.0
130.80	161.0
136.80	179.0
140.80	705.0
142.90	1385.0
144.90	714.0
147.80	181.0
154.90	200.0
156.80	115.0
160.70	110.0
170.80	226.0
172.00	865.0
173.00	845.0
174.00	55304.0
175.00	3819.0
176.00	53376.0
177.00	3143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB348