

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071923\
 Data File : VV031712.D
 Acq On : 19 Jul 2023 13:09
 Operator : SY/MD
 Sample : VSTD0.0532
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05232

Quant Time: Jul 20 04:59:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM071923.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 20 04:59:20 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	4893	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	4659	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2414	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	276	0.064	ug/L	0.00
4) 1,2-Dichloroethane-d4	4.969	65	285	0.089	ug/L	0.00
7) 1,2-Dichloropropane-d6	5.995	67	331	0.082	ug/L	0.00
8) Toluene-d8	7.253	98	550	0.069	ug/L	0.00
10) 1,1,2,2-Tetrachloroeth...	10.163	84	274	0.101	ug/L	0.02
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.280	62	290	0.040	ug/L #	71
6) Trichloroethene	5.852	95	200	0.048	ug/L	91
9) 1,2-Dibromoethane	8.305	107	126	0.051	ug/L #	79
12) 1,2,3-Trichloropropane	10.214	75	108	0.044	ug/L	96
13) 1,2-Dibromo-3-chloropr...	12.356	75	24	0.063	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071923\
Data File : VV031712.D
Acq On : 19 Jul 2023 13:09
Operator : SY/MD
Sample : VSTD0.0532
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05232

Quant Time: Jul 20 04:59:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM071923.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 20 04:59:20 2023
Response via : Initial Calibration

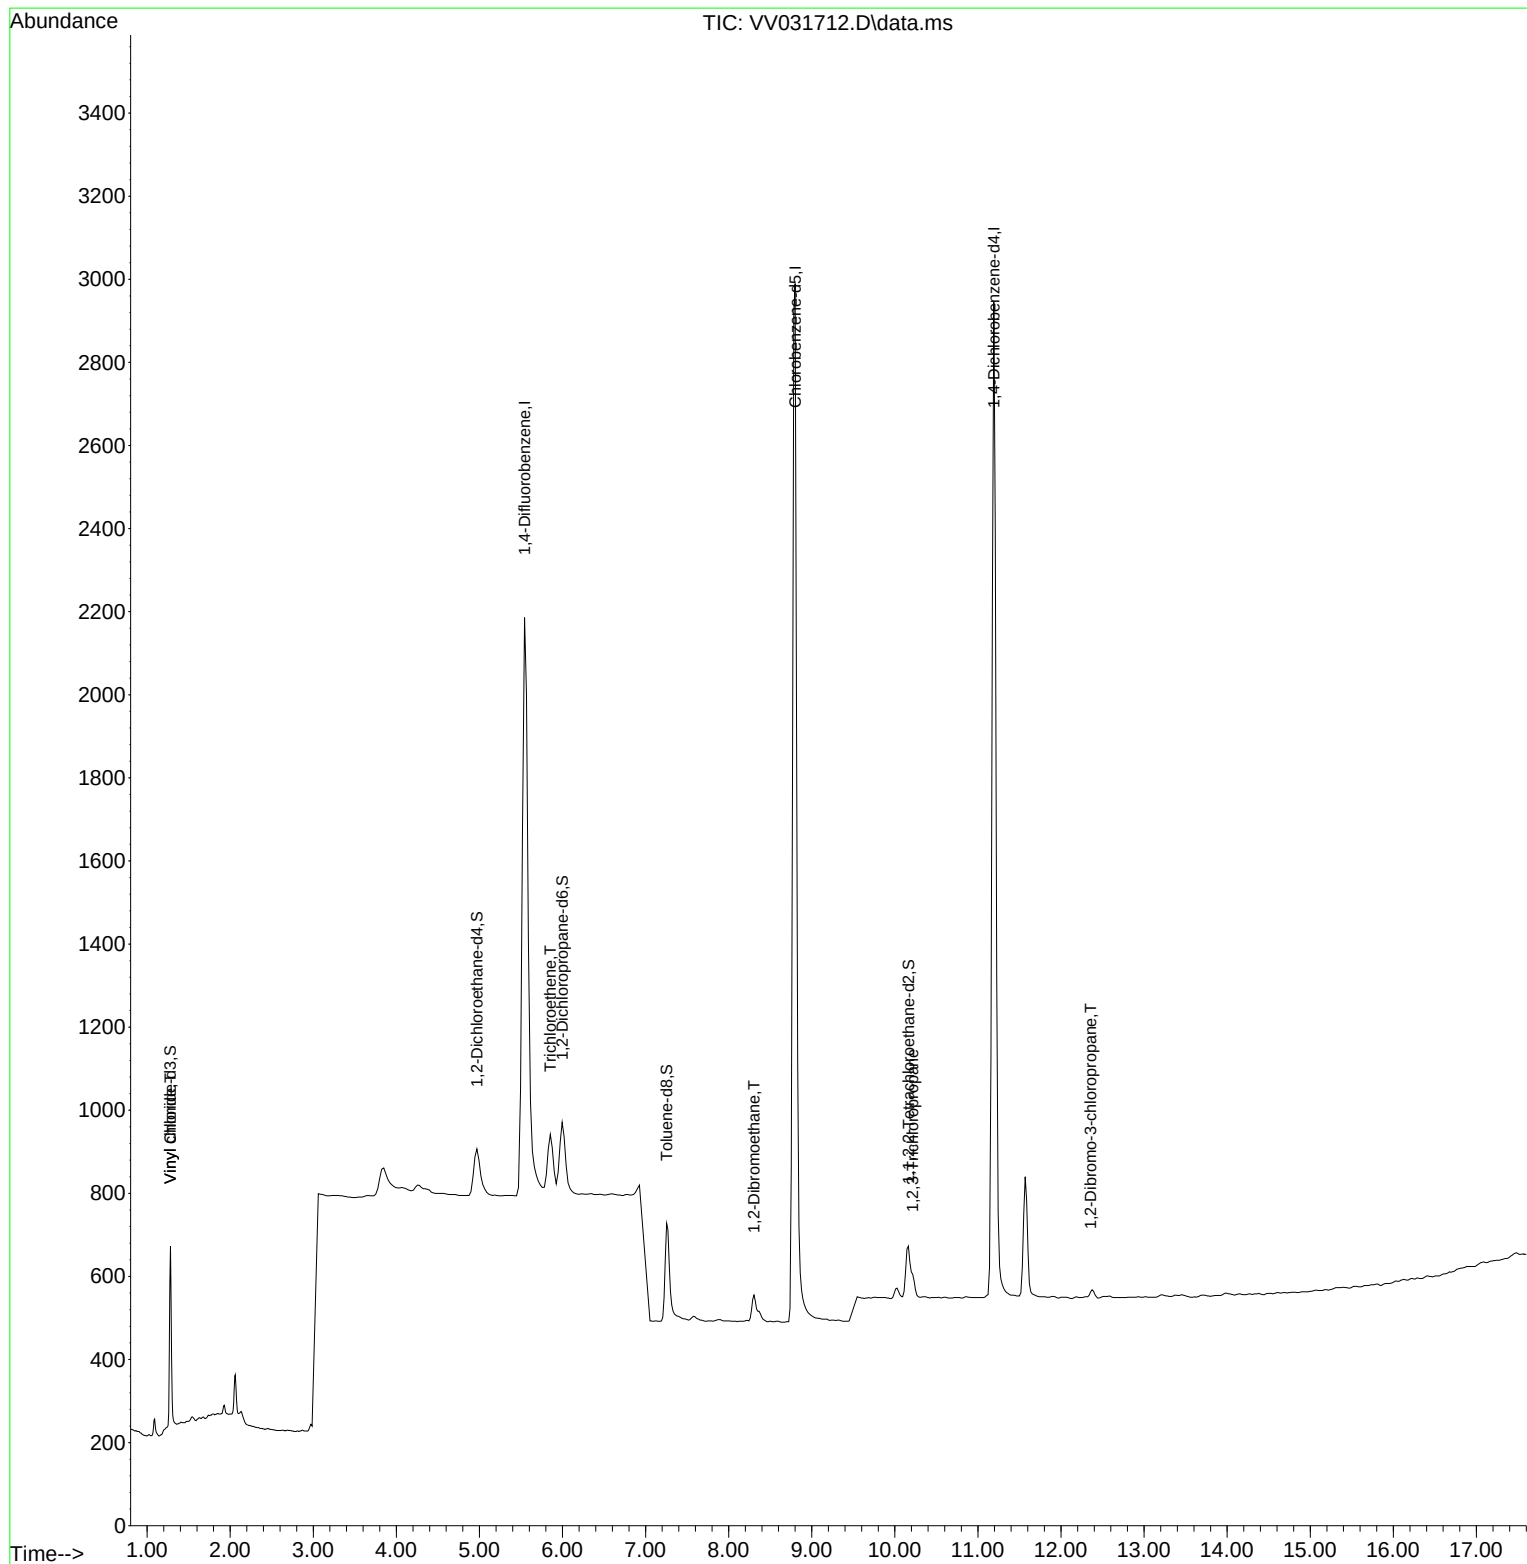

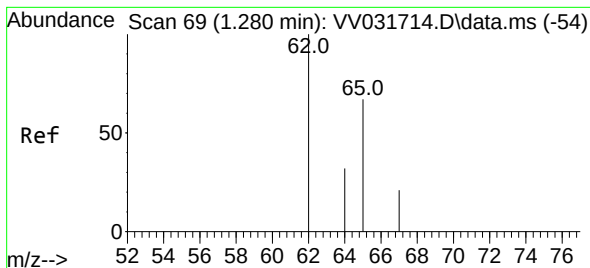

#3

Vinyl chloride

Concen: 0.040 ug/L

RT: 1.280 min Scan# 69

Delta R.T. -0.000 min

Lab File: VV031712.D

Acq: 19 Jul 2023 13:09

Instrument :

MSVOA_V

ClientSampleId :





VSTD0.05232

Tgt Ion: 62 Resp: 290

Ion Ratio Lower Upper

62 100

64 50.9 23.9 44.3#

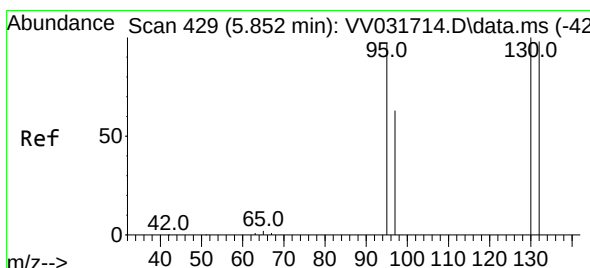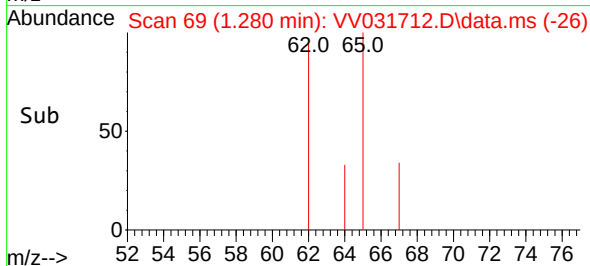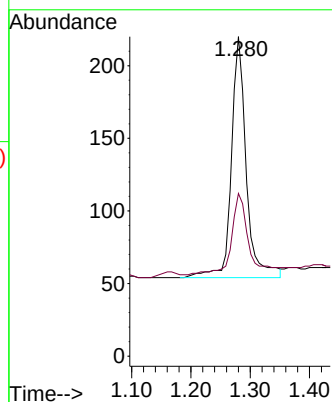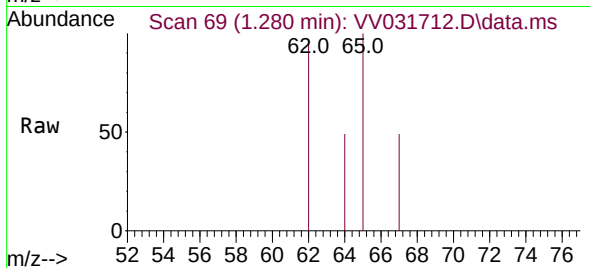

#6

Trichloroethene

Concen: 0.048 ug/L

RT: 5.852 min Scan# 429

Delta R.T. -0.000 min

Lab File: VV031712.D

Acq: 19 Jul 2023 13:09

Tgt Ion: 95 Resp: 200




Ion Ratio Lower Upper


95 100

97 83.9 48.8 90.6

132 94.6 70.3 130.7

130 96.8 71.7 133.1


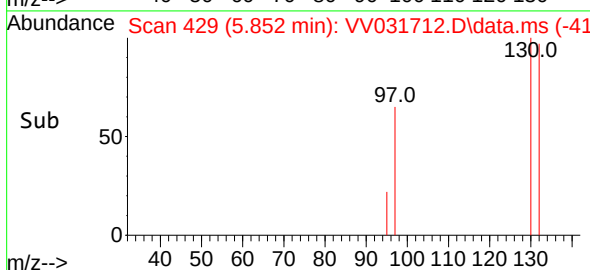
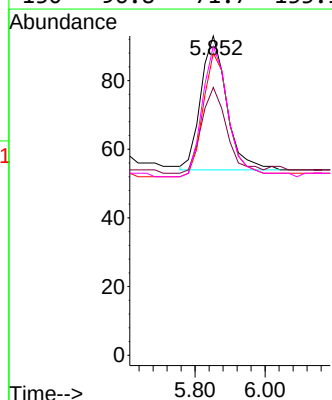
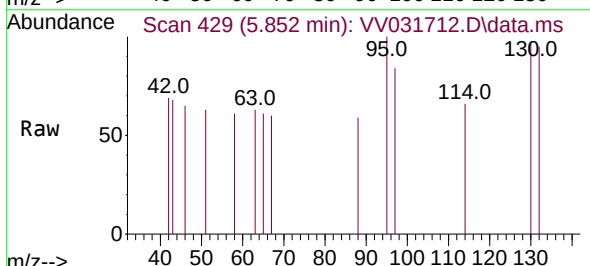


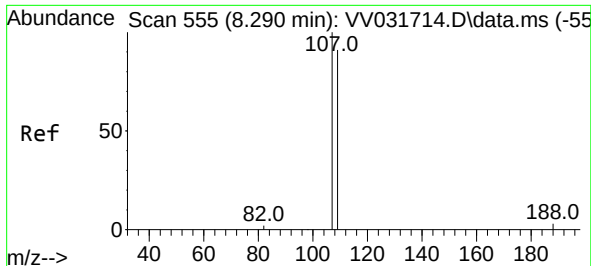

#9
1,2-Dibromoethane
Concen: 0.051 ug/L
RT: 8.305 min Scan# 511
Delta R.T. 0.015 min
Lab File: VV031712.D
Acq: 19 Jul 2023 13:09




Instrument :
MSVOA_V
ClientSampleId :
VSTD0.05232


Tgt Ion:107 Resp: 126
Ion Ratio Lower Upper
107 100
109 97.6 64.5 119.9
188 62.4 12.1 18.1#

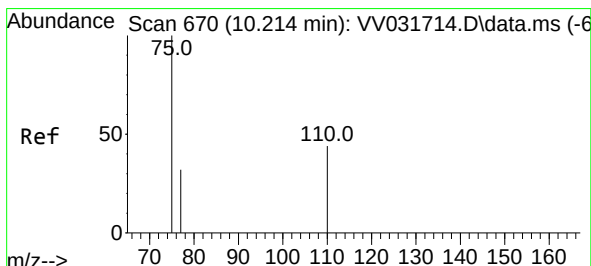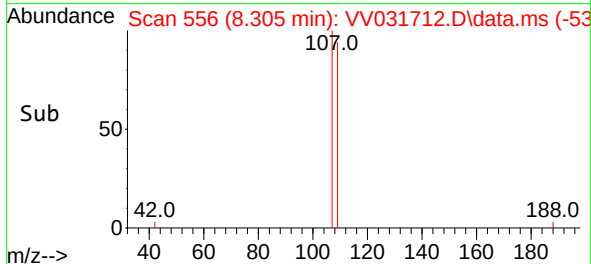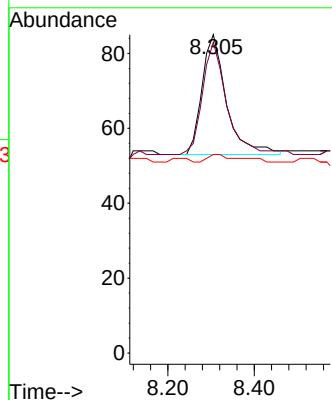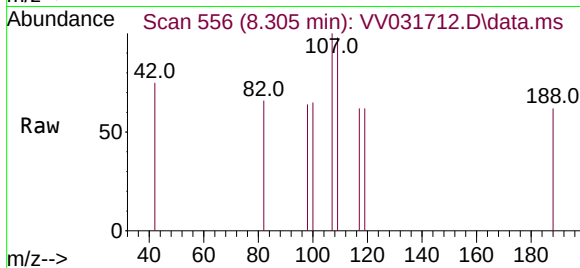

#12
1,2,3-Trichloropropane
Concen: 0.044 ug/L
RT: 10.214 min Scan# 670
Delta R.T. -0.000 min
Lab File: VV031712.D
Acq: 19 Jul 2023 13:09


Tgt Ion: 75 Resp: 108
Ion Ratio Lower Upper
75 100
110 40.7 33.4 50.2
77 37.0 26.1 39.1

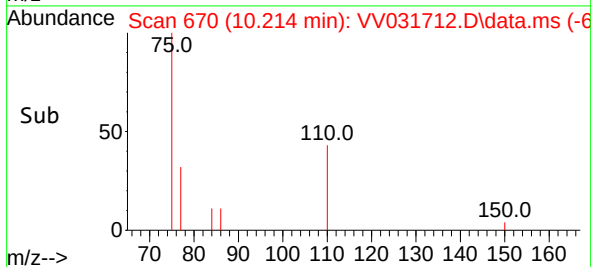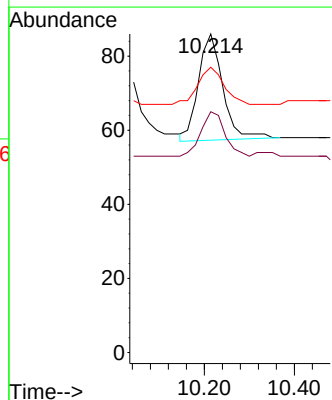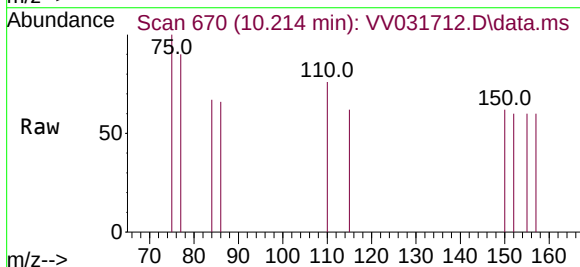

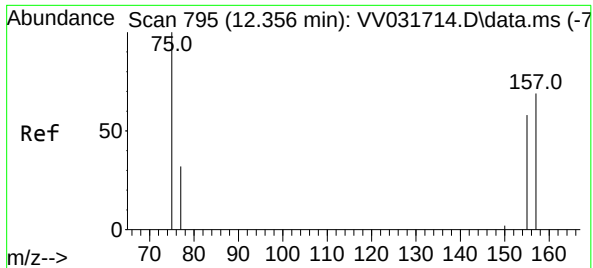

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.063 ug/L
 RT: 12.356 min Scan# 795
 Delta R.T. -0.000 min
 Lab File: VV031712.D
 Acq: 19 Jul 2023 13:09

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.05232

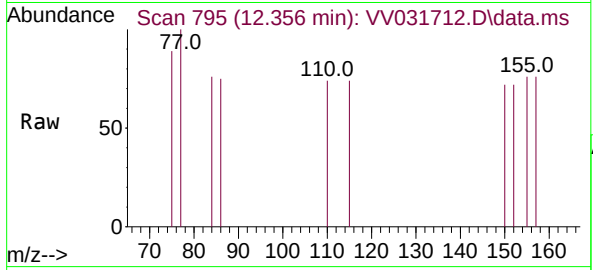

Tgt Ion: 75	Resp: 24
Ion Ratio	Lower Upper
75 100	
157 85.9	63.8 95.6
155 85.9	59.0 88.4

