

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071923\
 Data File : VV031717.D
 Acq On : 19 Jul 2023 15:51
 Operator : SY/MD
 Sample : VIBLK250
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK250

Quant Time: Jul 20 05:15:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM071923.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 20 05:08:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	4760	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	4601	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	2326	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	1924	0.508	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	4.969	65	1692	0.545	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
7) 1,2-Dichloropropane-d6	5.995	67	1938	0.520	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	104.000%
8) Toluene-d8	7.253	98	3030	0.494	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	1592	0.547	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	110.000%
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.356	75	12	0.027	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071923\
Data File : VV031717.D
Acq On : 19 Jul 2023 15:51
Operator : SY/MD
Sample : VIBLK250
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK250

Quant Time: Jul 20 05:15:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM071923.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 20 05:08:22 2023
Response via : Initial Calibration

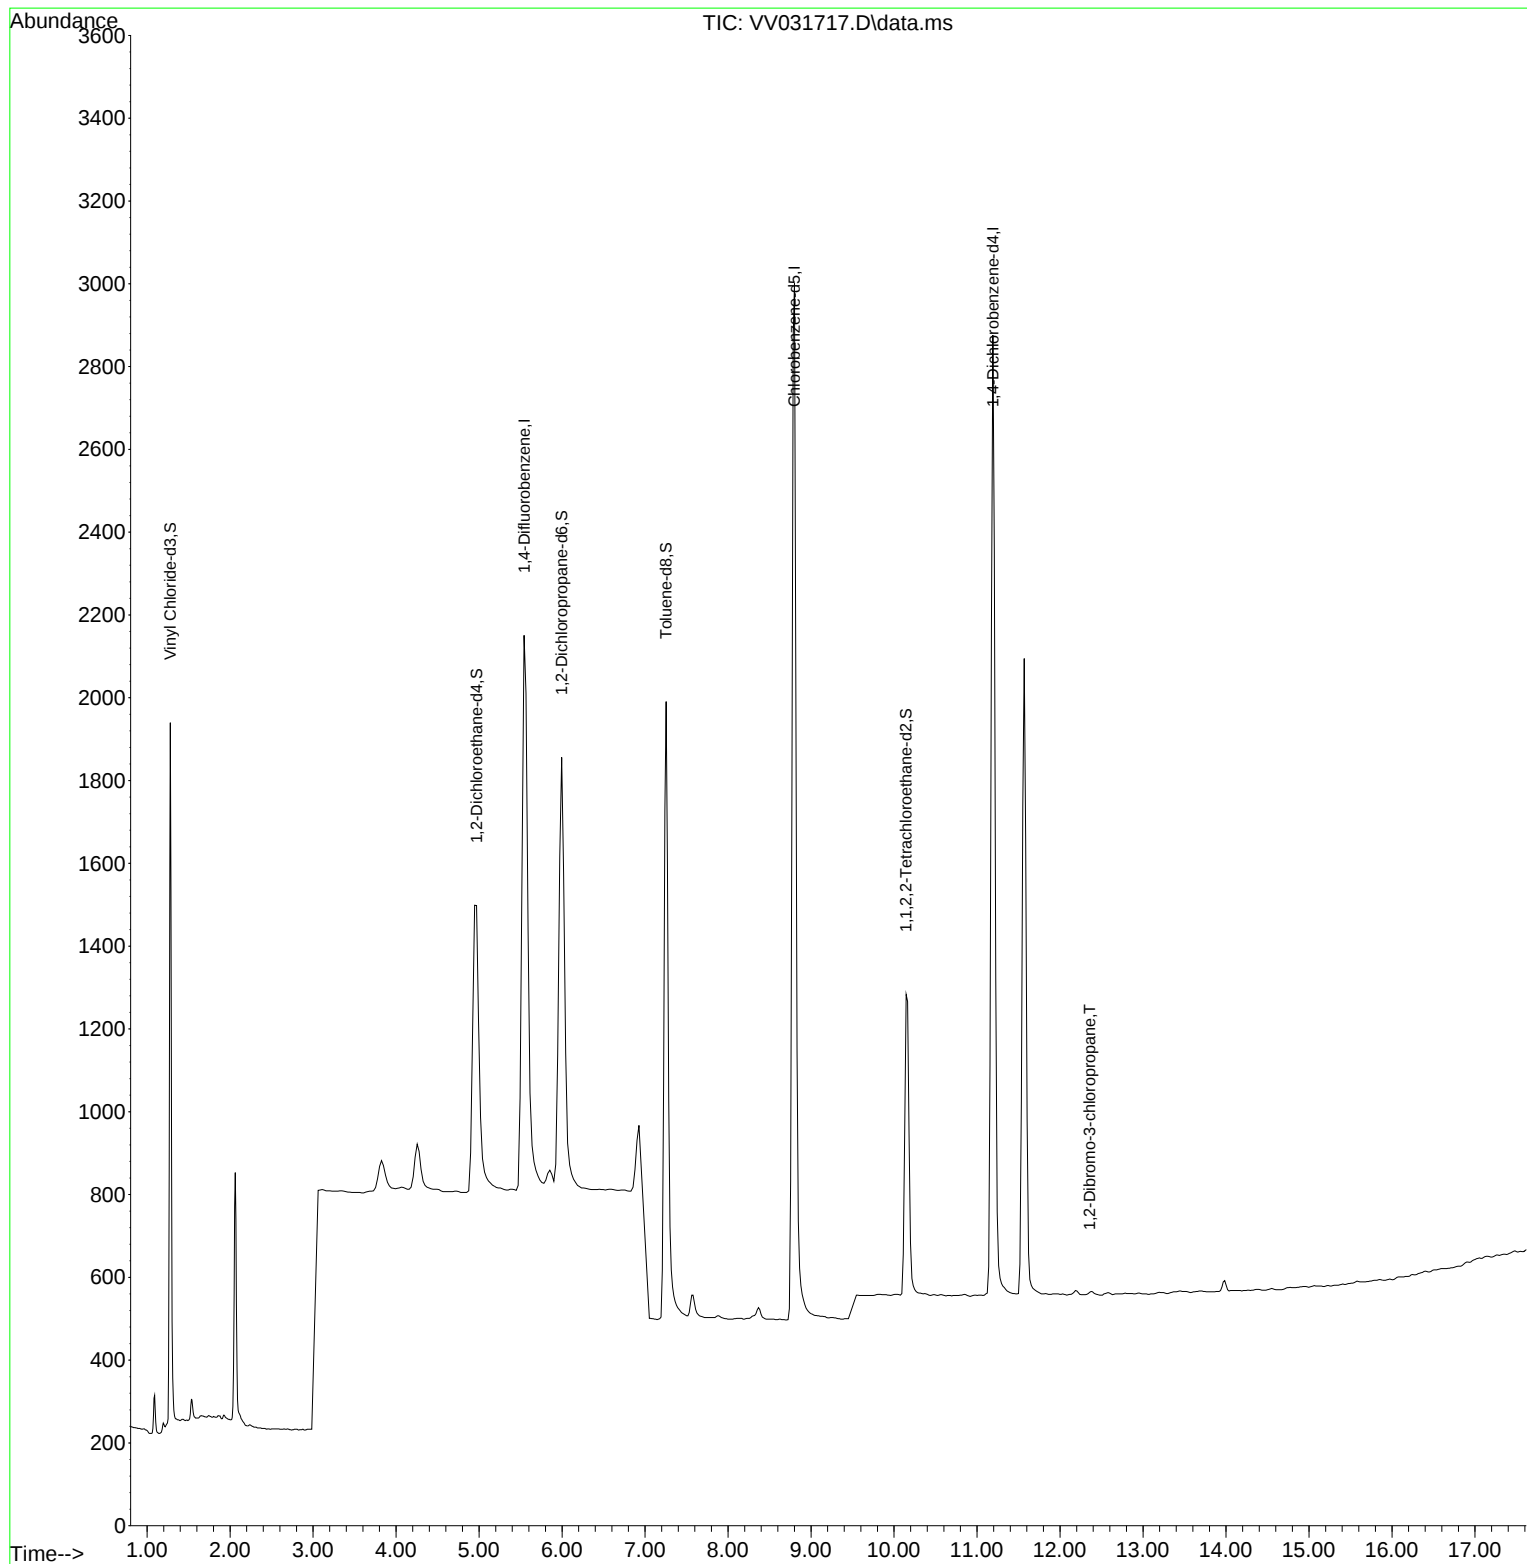

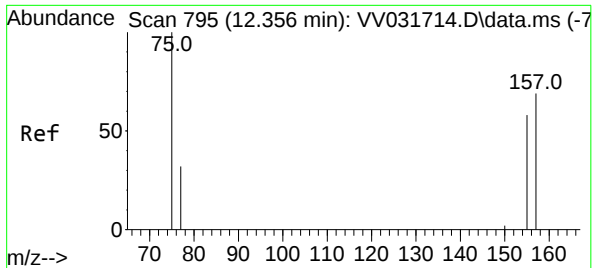

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.027 ug/L
 RT: 12.356 min Scan# 795
 Delta R.T. -0.000 min
 Lab File: VV031717.D
 Acq: 19 Jul 2023 15:51

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK250

Tgt Ion: 75	Resp:	12
Ion	Ratio	Lower Upper
75	100	
157	87.1	63.8 95.6
155	87.1	59.0 88.4

