
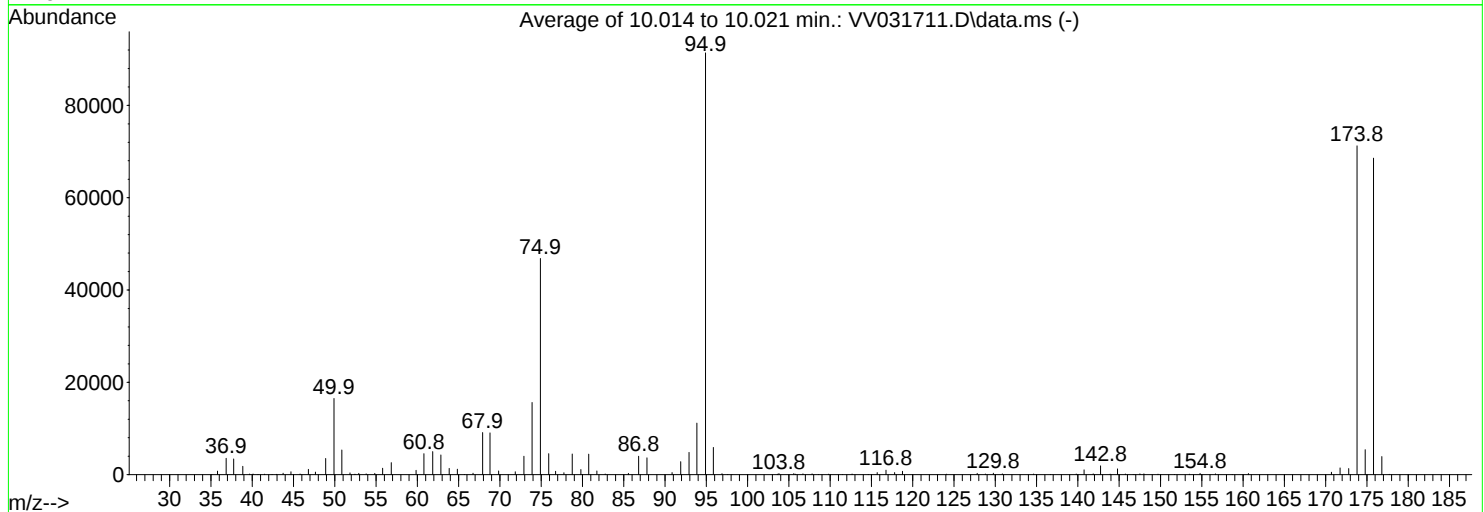


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV071923\
Data File : VV031711.D
Acq On : 19 Jul 2023 12:37
Operator : SY/MD
Sample : BFB241
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB241

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM071923.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jul 20 05:08:22 2023

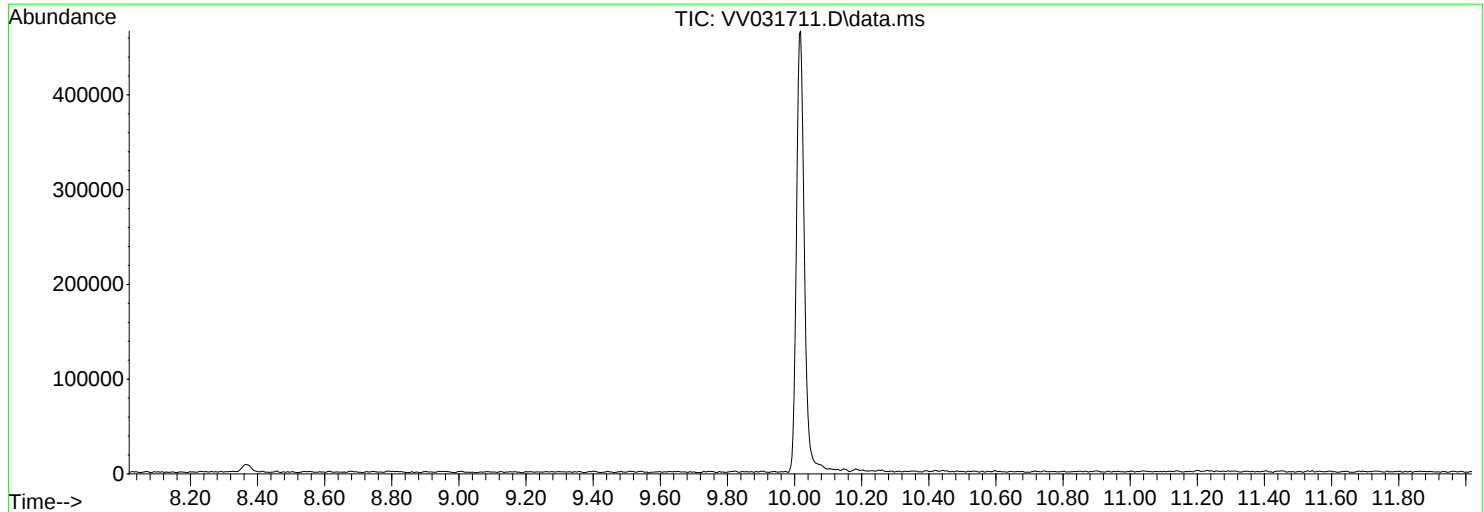

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	16515	PASS
75	95	30	80	51.2	46824	PASS
95	95	100	100	100.0	91389	PASS
96	95	5	9	6.5	5896	PASS
173	174	0.00	2	1.8	1316	PASS
174	95	50	120	77.9	71235	PASS
175	174	5	9	7.6	5405	PASS
176	174	95	101	96.3	68587	PASS
177	176	5	9	5.7	3926	PASS

m/z	Abundance
35.40	107.0
37.70	136.0
38.80	147.0
39.80	365.0
41.10	120.0
42.00	102.0
43.70	598.0
44.70	124.0
45.10	125.0
49.10	106.0
50.40	109.0
50.90	136.0
53.90	118.0
56.40	131.0
58.20	111.0
63.00	110.0
73.00	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
35.10	114.0
35.80	795.0
36.80	3822.0
37.80	3548.0
38.90	2161.0
39.70	536.0
42.90	129.0
43.80	870.0
44.70	654.0
45.70	178.0
46.80	1025.0
47.70	469.0
48.90	3628.0
49.90	17752.0
50.90	5808.0
51.90	409.0
52.50	147.0
52.90	226.0
53.80	258.0
54.90	306.0
55.80	1471.0
56.90	2761.0
59.80	983.0
60.80	4762.0
61.80	5335.0
62.90	4647.0
63.90	1483.0
64.80	1163.0
66.70	289.0
67.90	9389.0
68.80	9399.0
69.80	832.0
71.80	626.0
72.90	3856.0
73.90	16026.0
74.90	48752.0
75.90	5000.0
76.80	725.0
77.70	451.0
78.80	4547.0
79.80	1085.0
80.80	4386.0
81.70	805.0
82.80	140.0
85.50	200.0
86.80	4179.0
87.80	3495.0
90.80	496.0
91.90	2843.0
92.90	4837.0
93.90	11220.0
94.90	93776.0
95.90	6122.0
96.90	240.0
103.60	367.0
105.60	377.0
106.70	167.0
107.70	159.0
109.80	160.0
111.50	106.0
112.70	145.0
114.60	110.0
115.70	458.0
116.70	1042.0
117.80	484.0
118.70	775.0
127.80	238.0
128.80	136.0
129.70	352.0
130.90	211.0
134.60	154.0
136.70	139.0
139.90	102.0
140.70	1104.0
141.90	176.0
142.80	2079.0
144.00	117.0
144.80	1377.0
145.80	160.0
146.70	107.0
147.50	125.0
148.00	147.0
149.70	171.0
153.50	165.0
154.80	246.0
156.70	194.0
160.60	273.0
170.70	645.0
171.70	1521.0
172.80	1213.0
173.80	71360.0
174.80	5434.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

175.8068840.0

176.804079.0

177.70119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
35.80	802.0
36.80	3519.0
37.80	3661.0
38.90	2006.0
39.70	498.0
41.50	132.0
43.00	109.0
43.80	912.0
44.80	778.0
45.80	126.0
46.80	1206.0
47.70	588.0
48.90	3692.0
49.90	16984.0
50.80	5680.0
51.90	426.0
52.40	186.0
52.90	315.0
53.80	317.0
54.80	282.0
55.80	1451.0
56.90	2657.0
59.90	999.0
60.80	4616.0
61.80	5099.0
62.90	4423.0
63.90	1469.0
64.90	1251.0
66.70	299.0
67.90	9359.0
68.80	9263.0
69.80	817.0
71.80	626.0
72.90	4357.0
73.90	16016.0
74.90	47848.0
75.90	4678.0
76.80	738.0
77.70	431.0
78.70	4594.0
79.80	1195.0
80.70	4463.0
81.80	806.0
82.70	141.0
85.60	286.0
86.80	4167.0
87.80	3716.0
90.90	485.0
91.90	2915.0
92.90	5071.0
93.80	11609.0
94.90	94352.0
95.80	5993.0
96.90	210.0
103.80	370.0
105.60	360.0
106.70	197.0
107.80	145.0
109.80	141.0
112.70	150.0
115.70	492.0
116.70	1032.0
117.80	492.0
118.70	754.0
124.10	130.0
127.80	270.0
128.80	161.0
129.80	319.0
130.80	201.0
134.70	143.0
139.90	119.0
140.70	1033.0
141.90	174.0
142.80	1974.0
143.90	102.0
144.80	1308.0
145.80	133.0
147.50	182.0
148.00	174.0
149.70	144.0
153.50	115.0
154.80	299.0
156.70	210.0
160.70	245.0
170.70	510.0
171.80	1503.0
172.80	1351.0
173.80	73424.0
174.80	5498.0
175.80	70832.0
176.80	4024.0
177.70	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
35.80	667.0
36.90	3285.0
37.80	3379.0
38.90	1690.0
39.60	485.0
40.10	373.0
40.70	132.0
41.50	181.0
42.40	107.0
43.80	937.0
44.80	824.0
45.90	102.0
46.80	1212.0
47.60	607.0
48.90	3510.0
49.90	14810.0
50.80	4986.0
51.80	341.0
52.90	318.0
53.80	305.0
54.80	288.0
55.80	1289.0
56.80	2391.0
59.90	874.0
60.80	4277.0
61.90	4526.0
62.80	4095.0
63.80	1148.0
64.90	1180.0
65.70	127.0
66.80	328.0
67.90	8599.0
68.80	8532.0
69.90	750.0
71.90	598.0
72.90	4216.0
73.90	14851.0
74.90	43872.0
75.90	3916.0
76.70	698.0
77.80	358.0
78.70	4298.0
79.80	1095.0
80.70	4509.0
81.80	831.0
82.70	188.0
85.60	368.0
86.80	3669.0
87.80	3712.0
90.90	375.0
91.90	2638.0
92.90	4519.0
93.80	10705.0
94.90	86040.0
95.90	5573.0
96.90	231.0
97.60	108.0
98.10	101.0
103.80	417.0
105.80	362.0
106.70	158.0
107.90	178.0
108.60	124.0
112.60	126.0
115.70	383.0
116.80	841.0
117.80	428.0
118.80	700.0
124.10	136.0
127.80	325.0
128.80	174.0
129.70	271.0
130.80	142.0
134.70	149.0
139.70	152.0
140.80	962.0
141.70	180.0
142.70	1666.0
143.80	105.0
144.80	1011.0
145.70	124.0
146.90	100.0
147.50	215.0
148.00	211.0
151.70	103.0
154.80	305.0
156.60	162.0
158.70	104.0
160.70	198.0
170.80	375.0
171.80	1338.0
172.80	1384.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

173.80	68920.0
174.80	5282.0
175.80	66088.0
176.80	3675.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241