

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072018\
 Data File : VV006676.D
 Acq On : 20 Jul 2018 19:11
 Operator : SY/MD
 Sample : J4078-05
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA7

Quant Time: Jul 26 04:03:54 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jul 26 02:08:26 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	224387	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	205238	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	87406	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	78061	4.96	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.20%
7) Chloroethane-d5	1.58	69	59356	5.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.80%
11) 1,1-Dichloroethene-d2	2.13	63	114256	3.77	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.40%
20) 2-Butanone-d5	3.95	46	122484	35.81	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	71.62%
24) Chloroform-d	4.41	84	140030	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
26) 1,2-Dichloroethane-d4	5.09	65	68214	5.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.00%
32) Benzene-d6	5.10	84	298598	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.20%
36) 1,2-Dichloropropane-d6	6.12	67	93478	5.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.20%
41) Toluene-d8	7.36	98	260566	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
43) trans-1,3-Dichloropropene-	7.67	79	25203	4.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.00%
46) 2-Hexanone-d5	8.14	63	141570	48.41	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.82%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	65168	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	89053	5.66	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.20%


Target Compounds					Ovalue
13) Acetone	2.19	43	6155	2.35 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072018\
Data File : VV006676.D
Acq On : 20 Jul 2018 19:11
Operator : SY/MD
Sample : J4078-05
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA7

Quant Time: Jul 26 04:03:54 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jul 26 02:08:26 2018
Response via : Initial Calibration

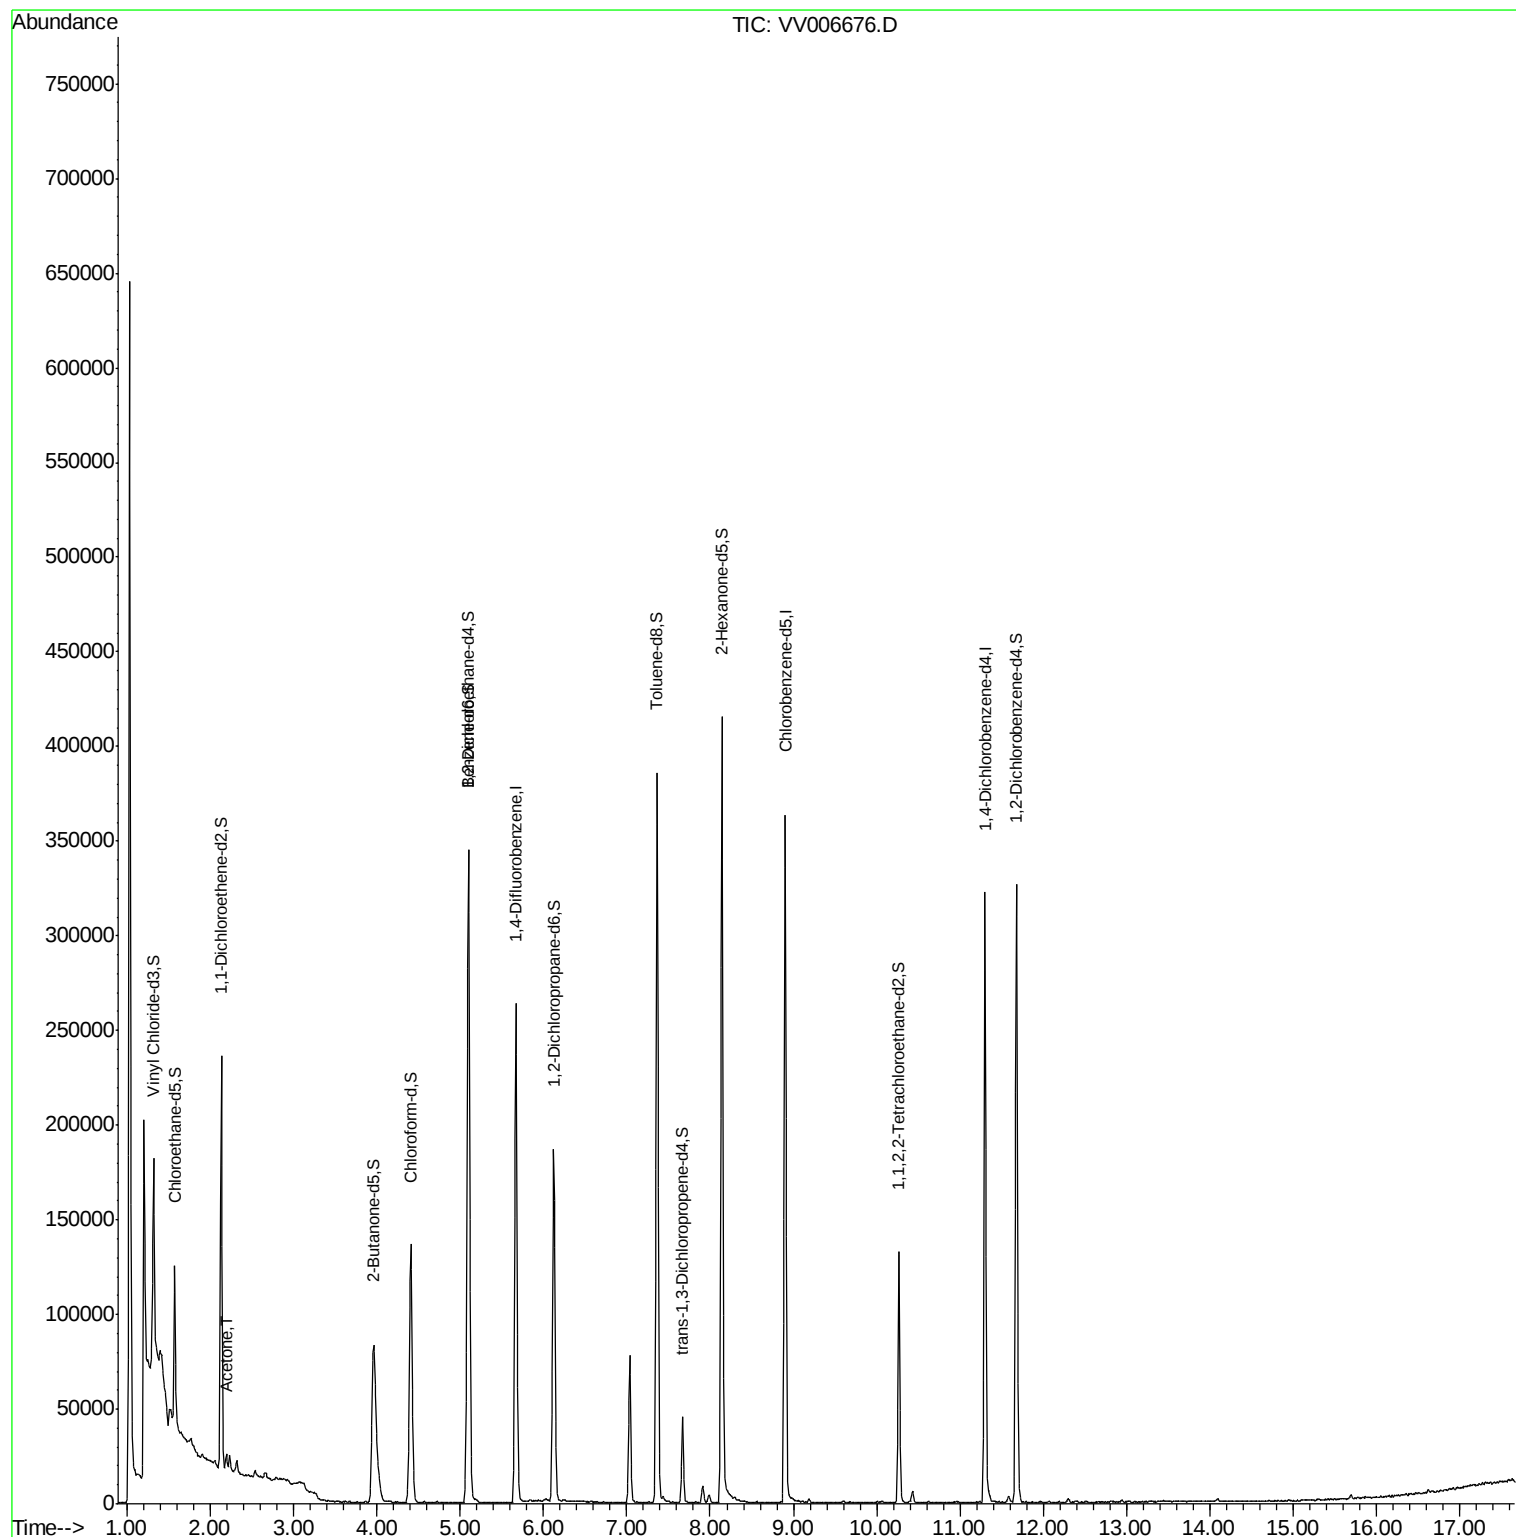

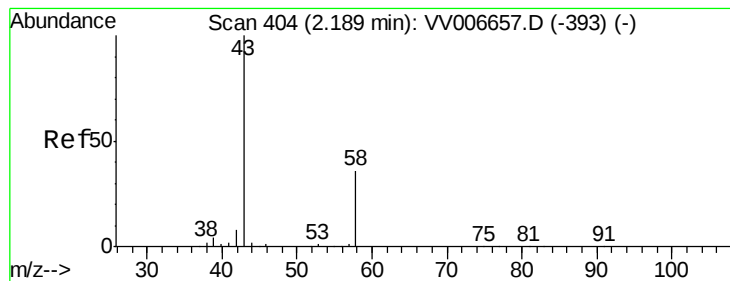

#13

Acetone

Concen: 2.35 ug/L

RT: 2.19 min Scan# 405

Delta R.T. 0.00 min

Lab File: VV006676.D

Acq: 20 Jul 2018 19:11


Instrument :
MSVOA_V
ClientSampleId :
C0AA7

Tot Ion: 43 Resp: 6155

Ion Ratio Lower Upper

43 100

58 36.6 0.0 72.8

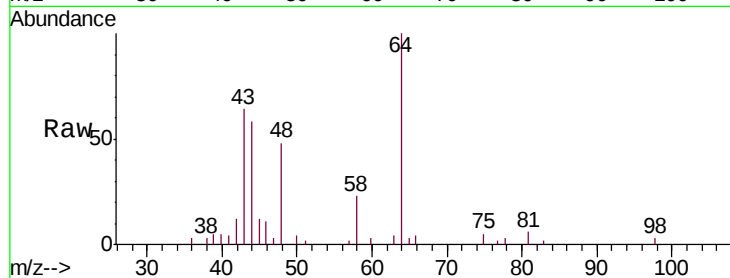

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

