


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072018\
Data File : VV006656.D
Acq On : 20 Jul 2018 07:37
Operator : SY/MD
Sample : BFB20
Misc : 25 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB20

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jul 26 14:13:27 2018

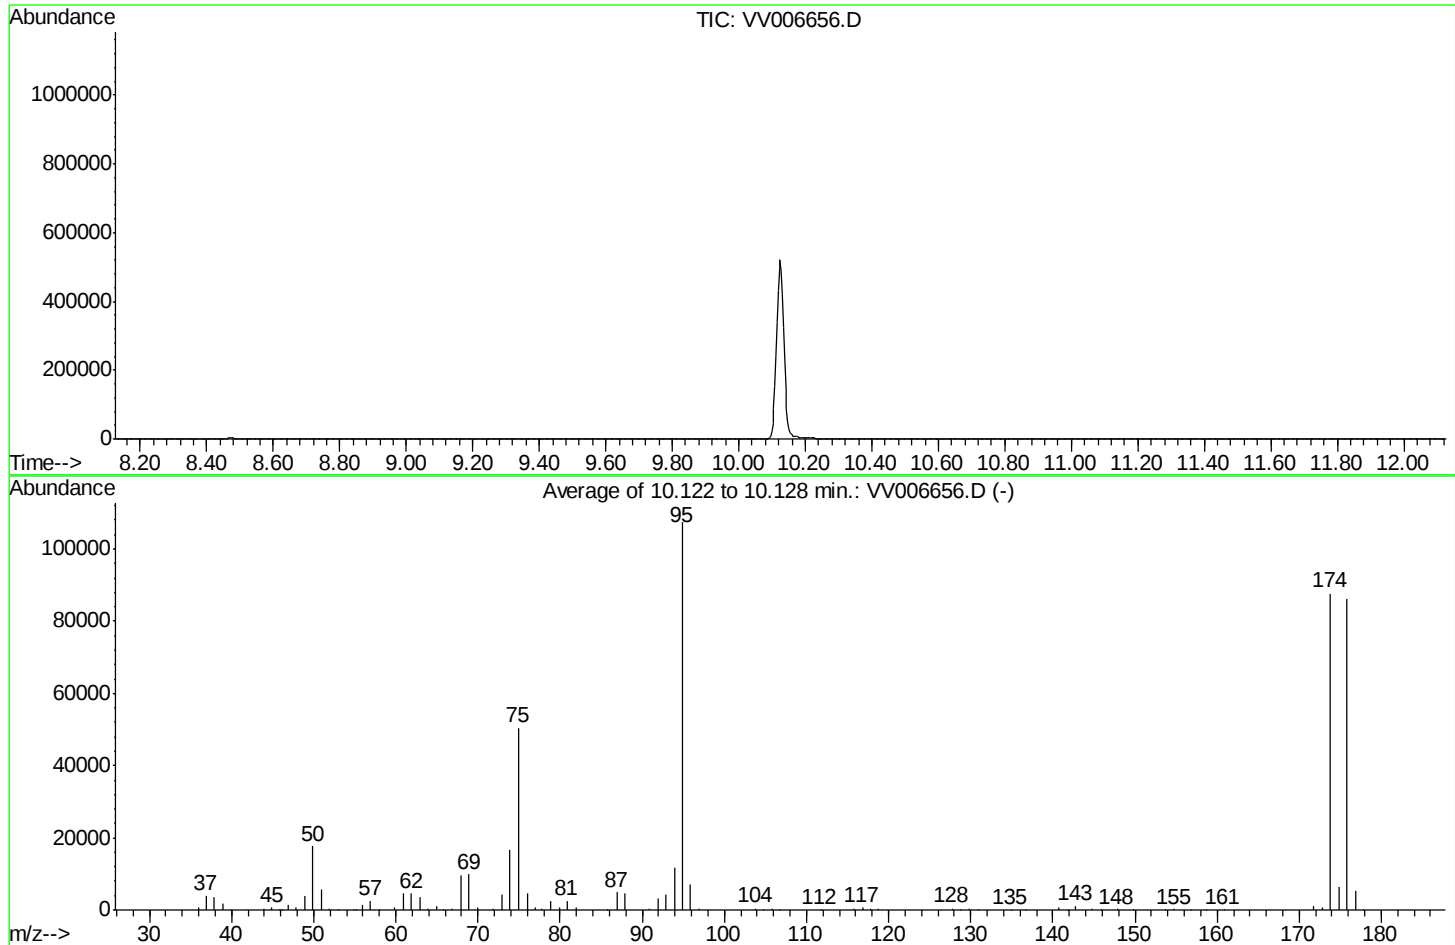

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	17656	PASS
75	95	30	80	47.0	50520	PASS
95	95	100	100	100.0	107400	PASS
96	95	5	9	6.6	7057	PASS
173	174	0.00	2	0.9	779	PASS
174	95	50	120	81.7	87701	PASS
175	174	5	9	7.1	6245	PASS
176	174	95	101	98.4	86309	PASS
177	176	5	9	6.1	5249	PASS

m/z	Abundance
39.80	131.0
43.90	618.0

Instrument :
MSVOA_V
ClientSampleId :
BFB20

m/z	Abundance
35.90	731.0
36.90	3999.0
37.90	3692.0
38.90	1825.0
39.90	253.0
44.00	905.0
44.90	722.0
46.00	110.0
46.90	1555.0
47.80	626.0
48.90	3831.0
49.90	17984.0
50.90	5705.0
51.90	276.0
54.80	264.0
55.90	1300.0
56.90	2546.0
57.90	160.0
59.90	933.0
60.90	4466.0
61.90	4568.0
62.90	3676.0
63.80	528.0
64.90	870.0
65.80	105.0
66.90	216.0
67.90	9780.0
68.90	10024.0
69.90	745.0
71.90	504.0
72.90	4397.0
73.90	16768.0
74.90	50384.0
76.00	4481.0
77.00	558.0
77.70	467.0
78.80	2537.0
79.90	911.0
80.80	2621.0
81.90	684.0
85.80	149.0
86.90	4870.0
87.80	4666.0
90.80	284.0
91.90	3006.0
92.90	4396.0
93.90	11588.0
94.90	106752.0
95.90	7304.0
97.00	227.0
103.80	456.0
104.80	167.0
105.80	375.0
106.80	126.0
115.90	296.0
116.80	587.0
117.80	409.0
118.80	552.0
127.80	375.0
128.80	127.0
129.80	341.0
130.90	140.0
134.90	144.0
136.70	125.0
140.80	845.0
141.80	122.0
142.80	1107.0
144.80	210.0
145.80	163.0
147.90	183.0
153.70	102.0
154.70	212.0
156.70	168.0
160.80	104.0
171.80	984.0
172.90	745.0
173.80	85064.0
174.90	6265.0
175.80	83088.0
176.90	5297.0
177.80	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB20

m/z	Abundance
35.90	720.0
36.90	4095.0
37.90	3824.0
38.90	1908.0
39.90	240.0
43.90	896.0
44.90	695.0
45.70	125.0
46.10	118.0
46.90	1518.0
47.80	628.0
48.90	3939.0
49.90	18232.0
50.90	5962.0
51.90	295.0
52.90	106.0
54.90	250.0
55.90	1378.0
56.90	2570.0
57.90	140.0
59.90	935.0
60.90	4564.0
61.90	4660.0
62.90	3783.0
63.80	547.0
64.90	963.0
65.80	103.0
66.90	239.0
67.90	10116.0
68.90	10166.0
69.90	825.0
71.90	525.0
72.90	4518.0
73.90	17224.0
74.90	52320.0
76.00	4606.0
76.90	620.0
77.70	463.0
78.80	2657.0
79.90	900.0
80.80	2735.0
81.90	697.0
85.70	167.0
86.90	5060.0
87.80	4745.0
90.80	294.0
91.90	3195.0
92.90	4550.0
93.90	12039.0
94.90	111168.0
95.90	7323.0
96.90	238.0
103.80	438.0
104.80	190.0
105.70	400.0
106.80	133.0
115.80	291.0
116.80	639.0
117.80	441.0
118.80	551.0
127.70	380.0
128.70	156.0
129.80	372.0
130.90	136.0
134.90	143.0
136.70	126.0
140.80	882.0
141.90	112.0
142.80	1128.0
144.70	224.0
145.80	152.0
147.90	210.0
149.80	105.0
153.70	110.0
154.80	198.0
156.70	180.0
158.70	107.0
171.80	1144.0
172.90	818.0
173.80	90608.0
174.90	6424.0
175.80	89568.0
176.90	5394.0
177.80	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB20

m/z	Abundance
35.90	653.0
36.90	3809.0
37.90	3503.0
38.90	1712.0
39.80	230.0
43.90	852.0
44.90	638.0
45.80	124.0
46.90	1314.0
47.80	577.0
48.90	3782.0
49.90	16752.0
50.90	5587.0
51.90	270.0
55.10	233.0
55.90	1310.0
56.90	2363.0
57.90	128.0
59.80	809.0
60.90	4325.0
61.90	4432.0
62.90	3516.0
63.80	517.0
64.90	931.0
66.90	244.0
67.90	9263.0
68.90	9409.0
69.90	785.0
71.90	480.0
72.90	4182.0
73.90	16063.0
74.90	48856.0
76.00	4308.0
76.90	634.0
77.70	402.0
78.80	2428.0
79.90	810.0
80.80	2570.0
81.90	682.0
85.70	178.0
86.90	4838.0
87.90	4436.0
90.80	308.0
91.90	3016.0
92.90	4243.0
93.90	11276.0
94.90	104280.0
95.90	6545.0
96.90	227.0
103.90	374.0
104.70	173.0
105.70	380.0
106.80	126.0
111.70	105.0
115.80	276.0
116.80	600.0
117.80	413.0
118.70	496.0
127.70	350.0
128.70	164.0
129.80	354.0
130.80	122.0
134.90	125.0
136.70	120.0
140.80	844.0
141.90	115.0
142.80	1005.0
144.70	209.0
145.80	151.0
147.80	215.0
154.90	193.0
156.80	184.0
158.70	103.0
171.80	1208.0
172.90	776.0
173.80	87432.0
174.90	6047.0
175.80	86272.0
176.80	5058.0
177.80	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB20