
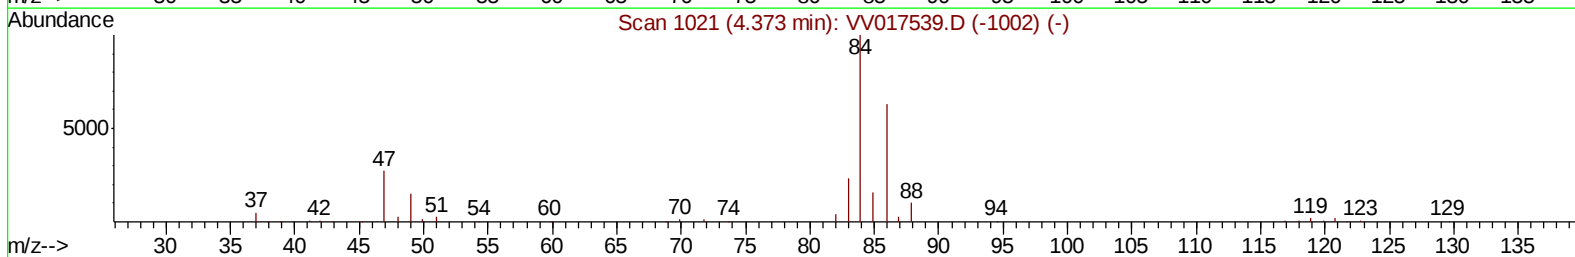
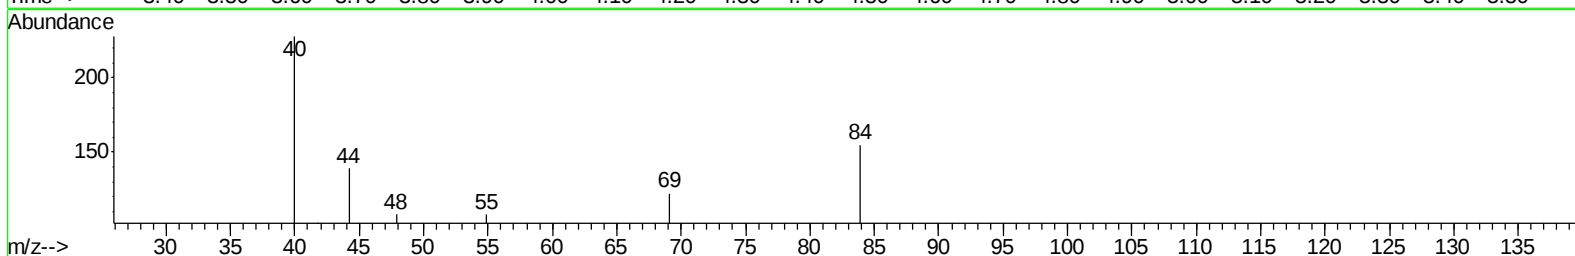


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072020\
 Data File : VV017554.D
 Acq On : 20 Jul 2020 18:56
 Operator : SY/MD
 Sample : L3336-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jul 21 01:47:39 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 20 18:07:44 2020
 Response via : Initial Calibration

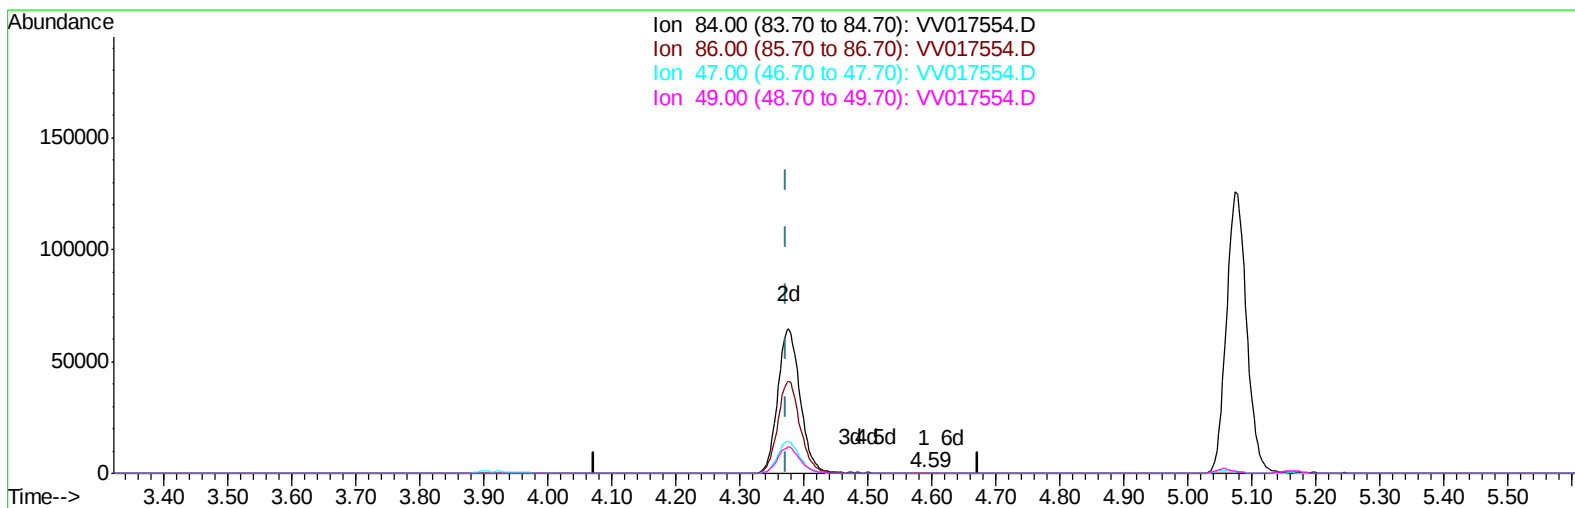

TIC: VV017554.D

(24) Chloroform-d (S)

4.589min (+0.215) 0.07ug/L

response 247

Ion	Exp%	Act%
84.00	100	100
86.00	62.50	56.28
47.00	46.70	41.70
49.00	27.20	20.65