


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV072020\
 Data File : VV017535.D
 Acq On : 20 Jul 2020 09:44
 Operator : SY/MD
 Sample : BFB63
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM072020WMA.M
 Title : VOC Analysis
 Last Update : Mon Jul 20 18:07:44 2020

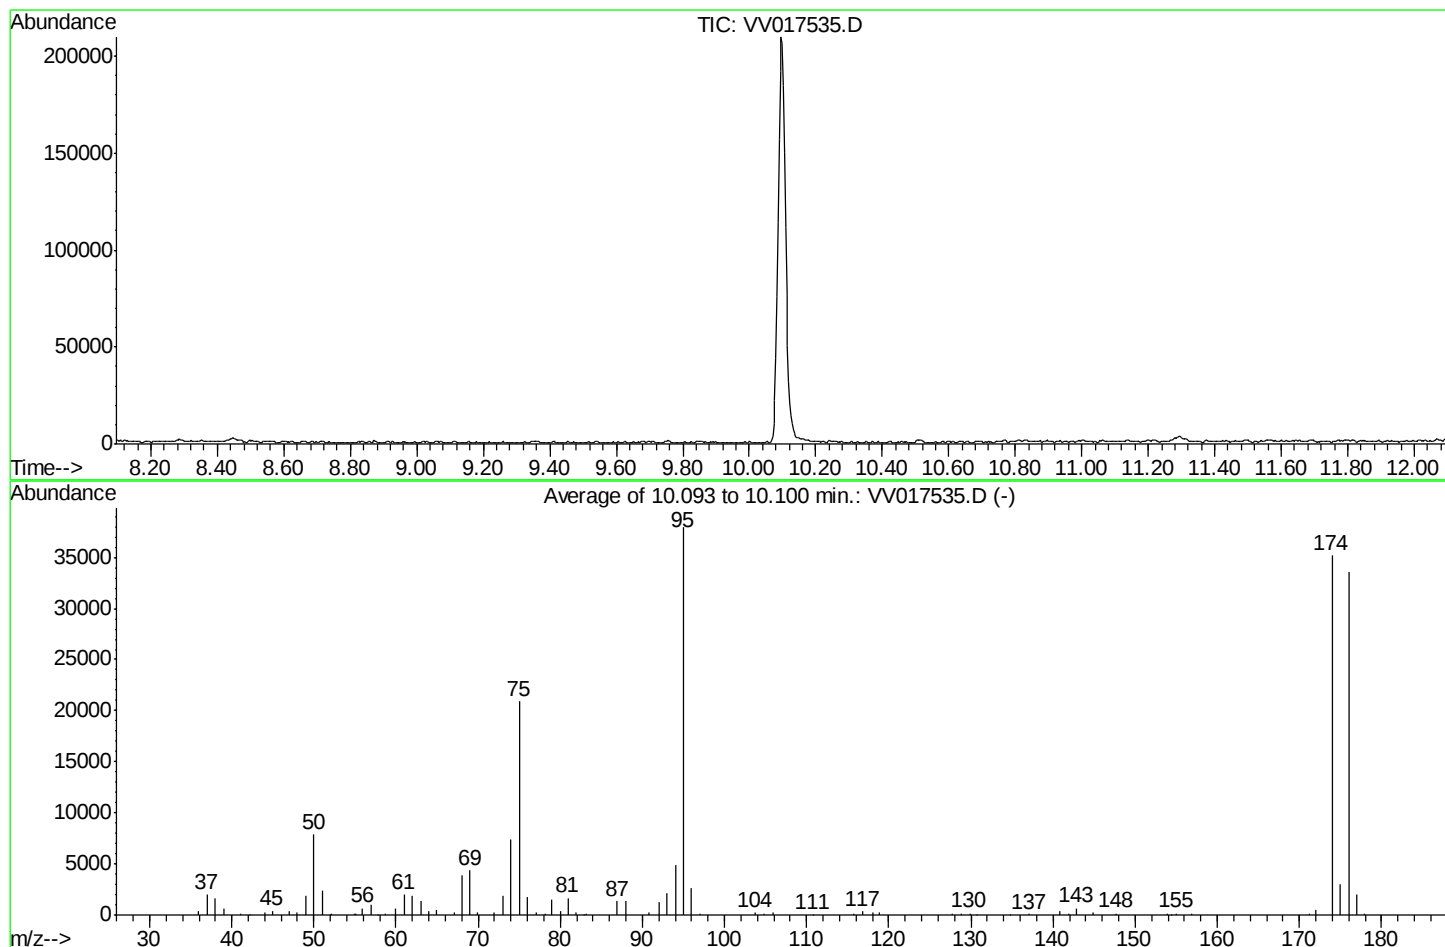

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	7860	PASS
75	95	30	80	55.1	20909	PASS
95	95	100	100	100.0	37944	PASS
96	95	5	9	6.9	2611	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.7	35157	PASS
175	174	5	9	8.7	3043	PASS
176	174	95	101	95.3	33520	PASS
177	176	5	9	6.1	2035	PASS

m/z	Abundance
35.90	347.0
37.00	1869.0
38.00	1725.0
39.00	622.0
39.90	223.0
42.20	122.0
43.90	402.0
44.90	445.0
47.00	388.0
47.90	238.0
49.00	1834.0
50.00	7725.0
51.00	2290.0
51.90	109.0
55.20	156.0
55.90	680.0
57.00	969.0
57.70	112.0
60.00	545.0
61.00	1920.0
62.00	1905.0
63.00	1408.0
64.00	381.0
64.90	451.0
67.10	205.0
68.00	3677.0
69.00	4400.0
69.90	252.0
72.00	210.0
73.10	1672.0
74.00	6903.0
75.00	20112.0
76.00	1737.0
77.00	211.0
78.10	206.0
78.90	1282.0
80.10	321.0
80.90	1538.0
81.90	211.0
82.80	119.0
87.00	1386.0
88.00	1379.0
90.90	252.0
92.00	1186.0
93.00	2025.0
94.00	4370.0
95.00	36856.0
96.00	2638.0
97.10	106.0
103.80	221.0
105.80	204.0
110.80	123.0
115.80	174.0
116.80	340.0
118.10	179.0
118.80	212.0
127.70	111.0
129.80	144.0
137.10	175.0
140.70	346.0
141.80	121.0
142.90	655.0
144.90	148.0
147.80	132.0
154.00	113.0
155.00	135.0
156.90	114.0
171.90	435.0
174.00	32664.0
174.90	3020.0
176.00	30432.0
177.00	1864.0
177.90	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
35.90	397.0
37.00	2163.0
38.00	1682.0
39.00	650.0
39.90	229.0
41.10	111.0
44.00	458.0
45.00	418.0
47.00	365.0
47.90	251.0
49.00	1968.0
50.00	8191.0
51.00	2430.0
52.20	100.0
55.10	173.0
55.90	720.0
57.00	1106.0
58.70	124.0
60.00	601.0
61.00	2047.0
62.00	1933.0
63.00	1413.0
64.00	396.0
65.00	480.0
67.10	200.0
68.00	4047.0
69.00	4515.0
70.00	318.0
71.90	234.0
73.10	1949.0
74.00	7689.0
75.00	21552.0
76.00	1734.0
77.10	221.0
78.90	1596.0
80.10	322.0
80.90	1752.0
81.90	251.0
83.20	122.0
86.90	1378.0
88.00	1424.0
90.80	289.0
92.00	1348.0
93.00	2287.0
94.00	5038.0
95.00	39200.0
96.00	2694.0
97.00	176.0
103.80	248.0
104.70	127.0
105.80	210.0
115.80	171.0
116.80	371.0
118.00	240.0
118.90	233.0
128.90	129.0
129.80	154.0
137.10	154.0
140.80	424.0
141.80	114.0
142.90	675.0
144.90	215.0
147.70	163.0
153.90	130.0
155.00	155.0
157.00	121.0
171.20	133.0
171.90	553.0
174.00	36496.0
174.90	3108.0
176.00	34648.0
177.00	2122.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	466.0
37.00	2175.0
38.00	1567.0
39.00	656.0
40.00	210.0
40.90	129.0
44.00	506.0
45.00	370.0
46.90	294.0
48.00	232.0
49.00	1726.0
50.00	7665.0
51.00	2324.0
52.20	126.0
54.90	207.0
56.00	668.0
57.00	1102.0
58.70	119.0
60.00	567.0
61.00	1992.0
62.00	1861.0
63.00	1375.0
64.00	331.0
65.00	450.0
67.10	189.0
68.00	4087.0
69.00	4146.0
70.00	348.0
72.00	241.0
73.00	2032.0
74.00	7511.0
75.00	21064.0
76.10	1708.0
77.10	266.0
78.90	1651.0
80.00	323.0
80.90	1615.0
81.90	263.0
83.20	107.0
86.90	1369.0
88.00	1314.0
90.80	243.0
92.00	1329.0
93.00	2268.0
94.00	5234.0
95.00	37776.0
96.00	2503.0
97.00	196.0
103.80	249.0
104.80	160.0
105.90	211.0
115.80	204.0
116.90	397.0
118.00	254.0
118.90	290.0
127.80	133.0
128.80	113.0
129.90	192.0
130.70	105.0
134.70	101.0
140.90	487.0
141.90	116.0
142.90	654.0
144.90	248.0
147.70	147.0
154.40	115.0
155.10	155.0
157.00	105.0
171.20	121.0
172.00	585.0
174.00	36312.0
174.90	3001.0
176.00	35480.0
177.00	2119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Scan 2790 (10.061 min): VV017535.D
BFB63

m/z	Abundance
36.80	116.0
40.10	275.0
44.00	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63