


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072021\
 Data File : VV021684.D
 Acq On : 20 Jul 2021 09:37
 Operator : SY/MD
 Sample : BFB208
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB208

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM071921WMA.M
 Title : VOC Analysis
 Last Update : Fri Jul 23 01:17:03 2021

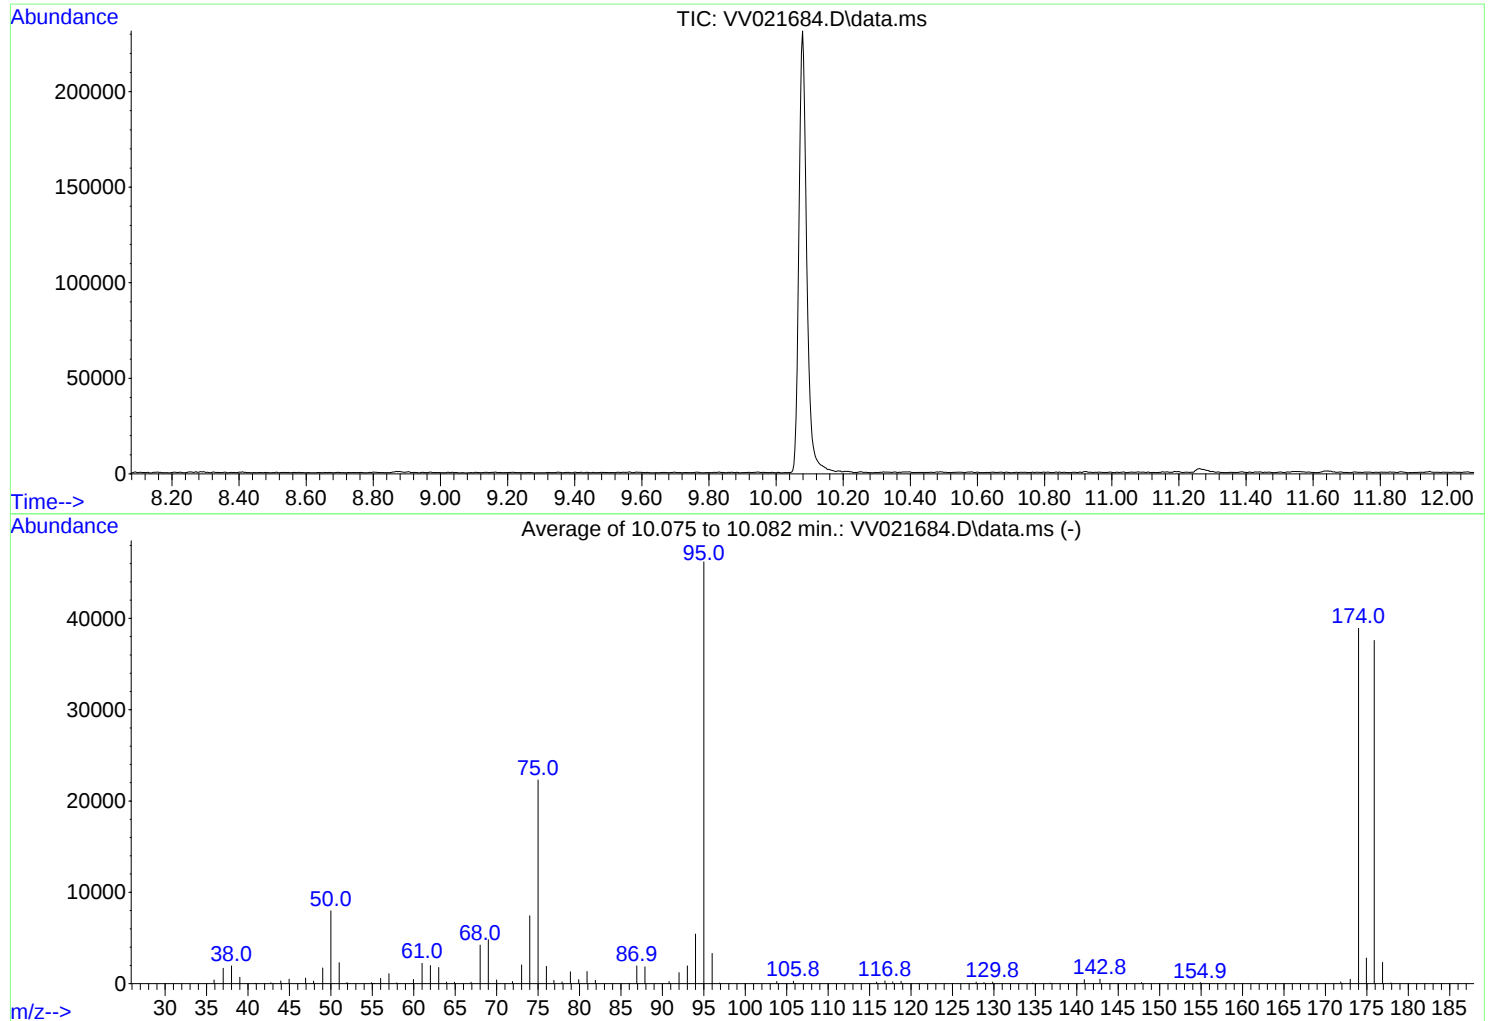

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	7982	PASS
75	95	30	80	48.3	22312	PASS
95	95	100	100	100.0	46192	PASS
96	95	5	9	7.2	3316	PASS
173	174	0.00	2	1.2	471	PASS
174	95	50	120	84.3	38923	PASS
175	174	5	9	7.2	2799	PASS
176	174	95	105	96.6	37589	PASS
177	176	5	10	6.2	2327	PASS

Scan 2800 (10.043 min): VV021684.D\data.ms
BFB208

m/z	Abundance
39.90	304.0
43.90	464.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
35.90	420.0
37.00	1646.0
38.00	1924.0
39.00	680.0
39.80	234.0
40.90	104.0
42.80	107.0
44.00	762.0
44.90	539.0
47.00	551.0
47.90	288.0
49.00	1729.0
50.00	8252.0
51.00	2328.0
51.90	125.0
54.90	115.0
56.00	541.0
57.00	1161.0
58.00	122.0
60.00	413.0
61.00	2055.0
62.00	2076.0
63.00	1749.0
63.90	175.0
64.90	166.0
66.90	160.0
68.00	4034.0
69.00	4827.0
70.00	371.0
71.90	192.0
73.00	2038.0
74.00	7444.0
75.00	22296.0
76.00	1867.0
76.90	325.0
77.80	237.0
78.90	1289.0
79.90	423.0
80.90	1315.0
81.90	376.0
86.90	1955.0
87.90	1785.0
90.80	230.0
92.00	1113.0
93.00	1962.0
94.00	5469.0
95.00	46032.0
96.00	3410.0
96.90	110.0
103.80	265.0
105.80	267.0
115.80	167.0
116.90	299.0
117.80	244.0
118.80	232.0
127.90	168.0
128.80	110.0
129.90	172.0
134.70	107.0
136.80	113.0
140.90	439.0
142.80	484.0
147.80	135.0
154.90	111.0
171.90	152.0
173.00	462.0
174.00	37320.0
175.00	2765.0
175.90	36280.0
176.90	2172.0
177.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
35.90	407.0
37.00	1737.0
38.00	2069.0
39.00	707.0
39.80	257.0
42.70	108.0
44.00	797.0
45.00	494.0
46.90	635.0
47.90	305.0
49.00	1799.0
50.00	8211.0
51.00	2326.0
51.90	120.0
54.90	105.0
56.00	602.0
57.00	1098.0
57.90	118.0
60.00	454.0
61.00	2354.0
62.00	2053.0
63.00	1822.0
64.00	174.0
64.90	179.0
66.90	177.0
68.00	4338.0
69.00	4973.0
70.00	438.0
71.90	227.0
73.00	2173.0
74.00	7713.0
75.00	23048.0
76.00	1970.0
76.90	363.0
77.90	190.0
78.90	1345.0
79.90	440.0
80.90	1363.0
81.90	360.0
86.00	107.0
86.90	1997.0
87.90	1888.0
90.80	239.0
92.00	1233.0
93.00	2012.0
94.00	5591.0
95.00	47872.0
96.00	3475.0
96.90	114.0
103.80	243.0
105.80	272.0
115.90	183.0
116.90	314.0
117.80	185.0
118.80	282.0
127.90	183.0
128.80	128.0
129.90	190.0
134.70	123.0
136.80	105.0
140.90	453.0
142.80	476.0
147.70	125.0
154.90	134.0
171.80	189.0
173.00	505.0
174.00	40480.0
174.90	2876.0
175.90	39128.0
176.90	2423.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
35.90	375.0
37.00	1690.0
38.00	1844.0
39.00	729.0
39.80	257.0
42.70	102.0
44.00	754.0
45.00	422.0
46.90	657.0
47.90	251.0
49.00	1623.0
50.00	7483.0
51.00	2249.0
52.00	108.0
54.90	110.0
55.20	111.0
56.00	609.0
57.00	1019.0
59.90	481.0
61.00	2290.0
62.00	1821.0
63.00	1728.0
64.00	164.0
64.90	153.0
66.90	151.0
68.00	4276.0
69.00	4659.0
70.00	411.0
71.90	263.0
73.00	1919.0
74.00	7125.0
75.00	21592.0
76.00	1860.0
76.90	364.0
78.00	150.0
78.90	1279.0
79.90	431.0
80.90	1301.0
81.90	346.0
86.90	1875.0
87.90	1823.0
90.80	203.0
92.00	1262.0
93.00	1884.0
94.00	5218.0
95.00	44672.0
96.00	3063.0
103.80	205.0
105.80	257.0
115.90	175.0
116.80	298.0
117.80	141.0
118.80	274.0
127.80	181.0
128.80	132.0
129.80	188.0
140.90	418.0
142.80	498.0
147.90	117.0
154.90	130.0
171.90	230.0
173.00	446.0
174.00	38968.0
174.90	2756.0
175.90	37360.0
176.90	2385.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208