
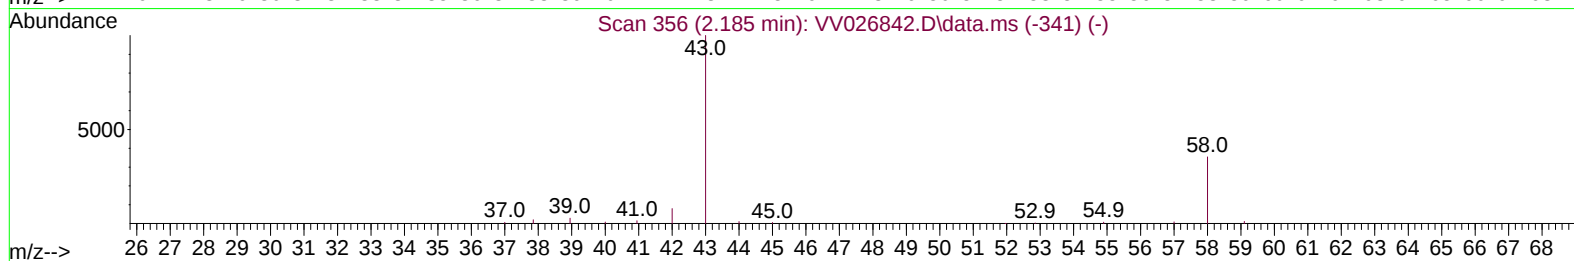
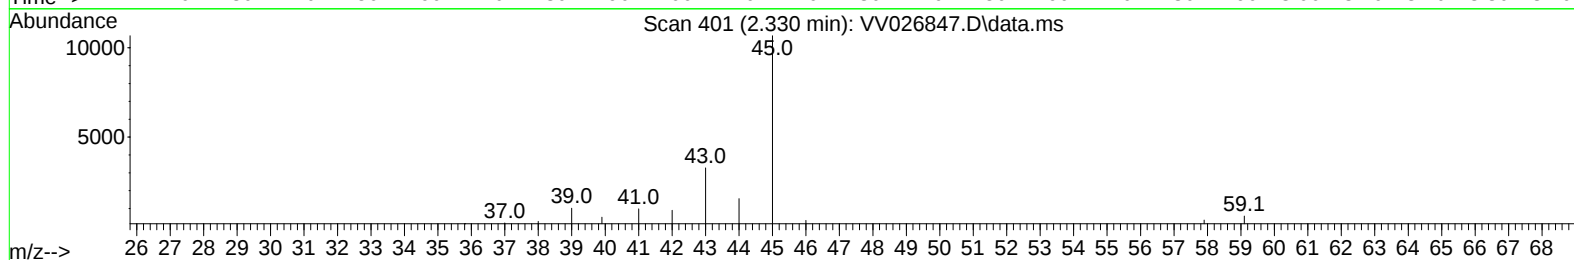


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026847.D
Acq On : 20 Jul 2022 12:18
Operator : SY/MD
Sample : N3754-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jul 21 01:49:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 21 01:47:16 2022
Response via : Initial Calibration

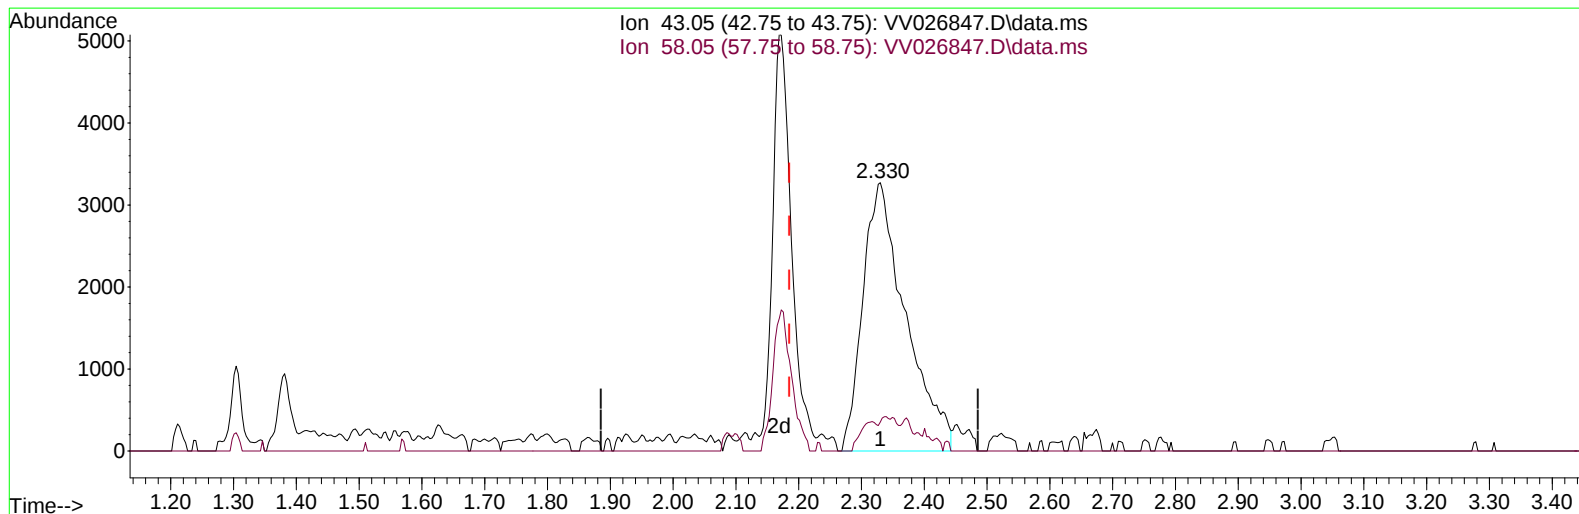

TIC: VV026847.D\data.ms

(13) Acetone (T)

2.330min (+ 0.145) 6.11 ug/L

response 15475

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	10.30	5.17
0.00	0.00	0.00
0.00	0.00	0.00