




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072022\  
Data File : VV026847.D  
Acq On : 20 Jul 2022 12:18  
Operator : SY/MD  
Sample : N3754-15  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
GBHQ7

Manual IntegrationsAPPROVED

Quant Time: Jul 21 01:49:56 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR071122WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Jul 21 01:47:16 2022  
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022  
Supervised By :Semsettin Yesilyurt 07/22/2022

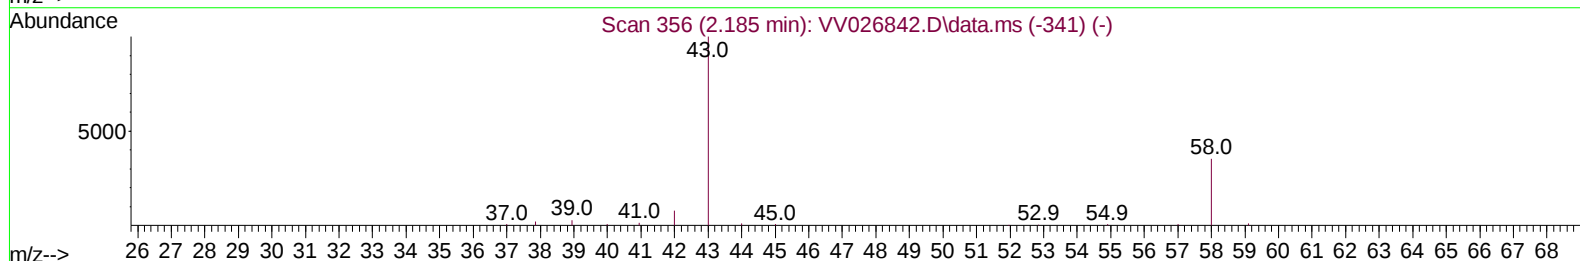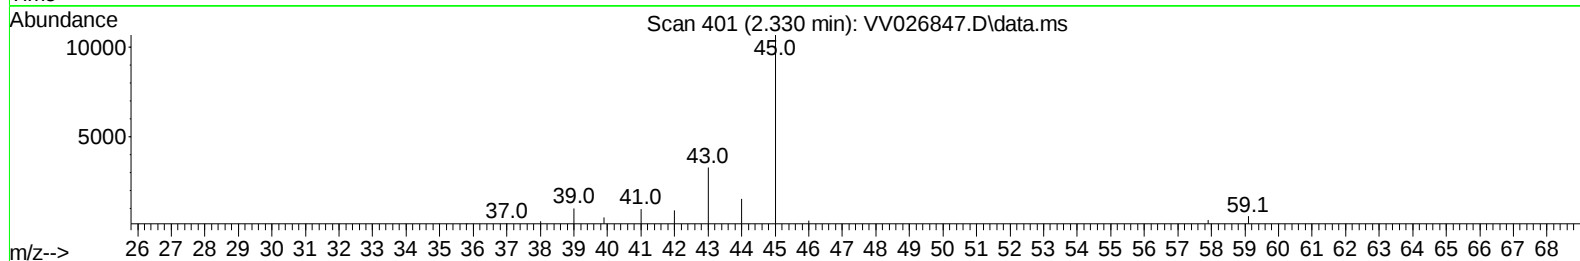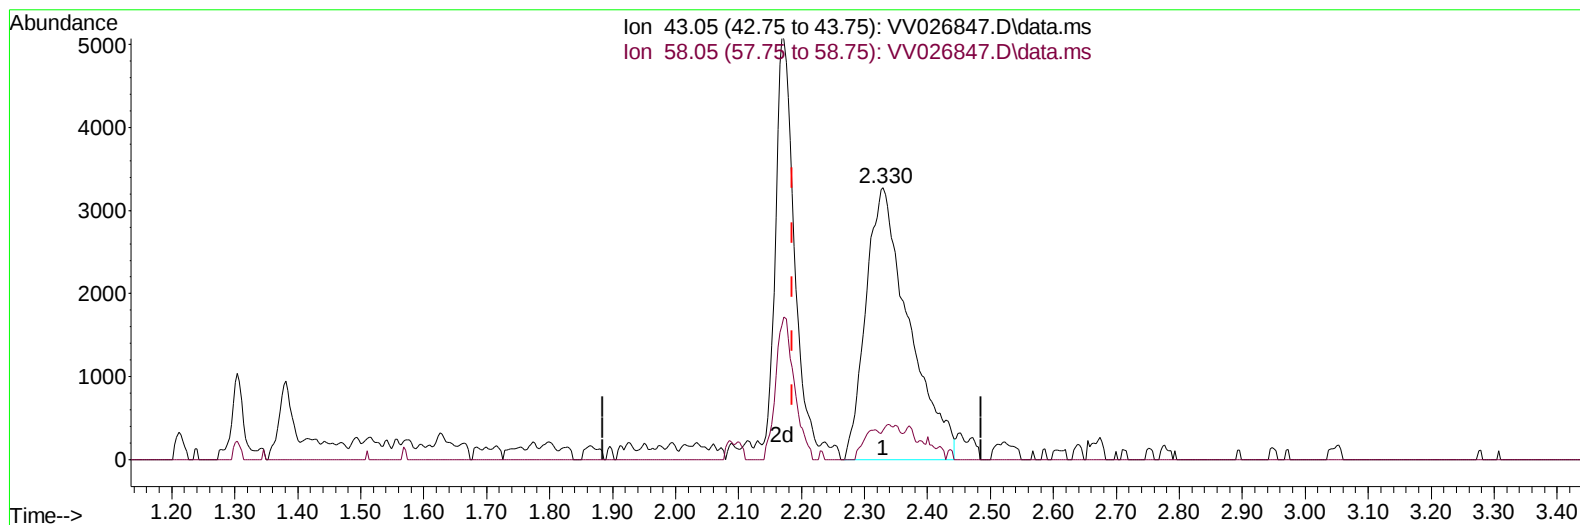

TIC: VV026847.D\data.ms

(13) Acetone (T)

2.330min (+ 0.145) 6.11 ug/L

response 15475

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 10.30  | 5.17   |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072022\  
Data File : VV026847.D  
Acq On : 20 Jul 2022 12:18  
Operator : SY/MD  
Sample : N3754-15  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
GBHQ7

## Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/22/2022  
Supervised By :Semsettin Yesilyurt 07/22/2022

Quant Time: Jul 21 01:49:56 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR071122WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Jul 21 01:47:16 2022  
Response via : Initial Calibration

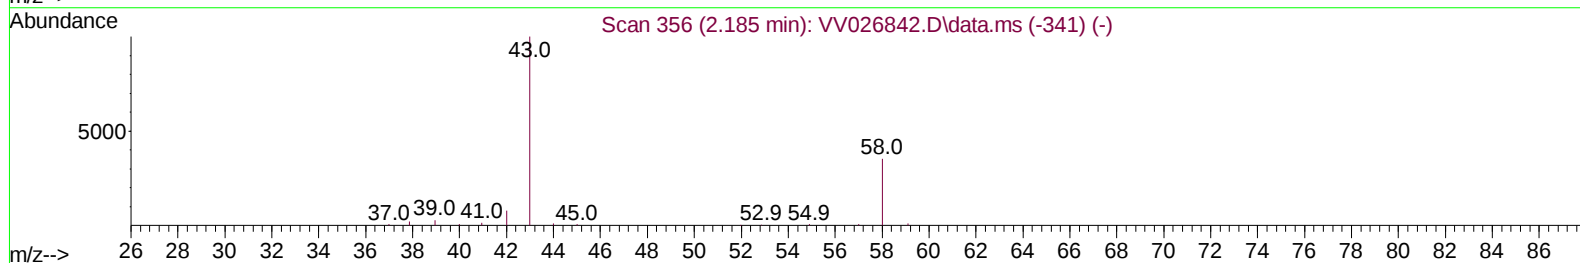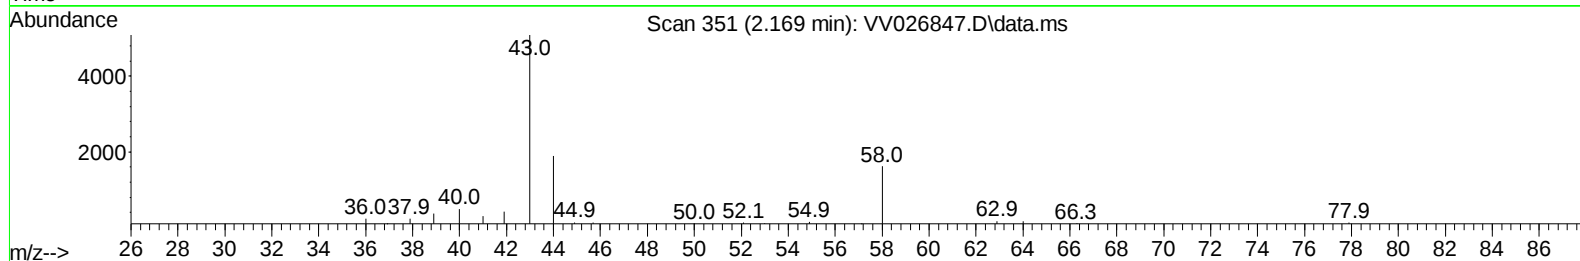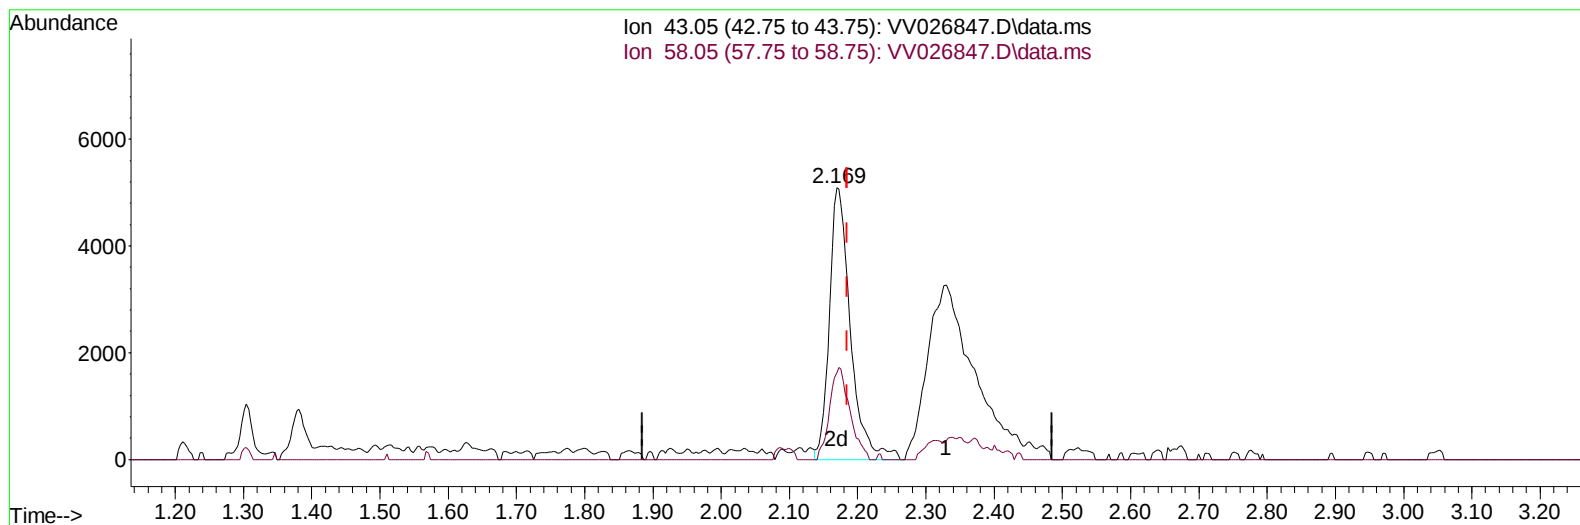

TIC: VV026847.D\data.ms

## (13) Acetone (T)

2.169min (-0.016) 4.31 ug/L m

response 10916

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 10.30  | 7.33   |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072022\  
 Data File : VV026847.D  
 Acq On : 20 Jul 2022 12:18  
 Operator : SY/MD  
 Sample : N3754-15  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 GBHQ7

## Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/22/2022  
 Supervised By :Semsettin Yesilyurt 07/22/2022

Quant Time: Jul 21 01:49:56 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR071122WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Jul 21 01:47:16 2022  
 Response via : Initial Calibration

| Compound                      | R.T.   | Q     | Ion      | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|----------|
| -----                         |        |       |          |          |        |          |          |
| Internal Standards            |        |       |          |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 5.616  | 114   |          | 211288   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 8.850  | 117   |          | 222155   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152   |          | 92090    | 5.000  | ug/L     | 0.00     |
| System Monitoring Compounds   |        |       |          |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.301  | 65    |          | 64355    | 3.339  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 66.800%  |          |
| 7) Chloroethane-d5            | 1.565  | 69    |          | 66119    | 3.970  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 79.400%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.102  | 63    |          | 88693    | 2.397  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 48.000%# |          |
| 20) 2-Butanone-d5             | 3.883  | 46    |          | 190050   | 63.173 | ug/L     | -0.01    |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 126.340% |          |
| 24) Chloroform-d              | 4.346  | 84    |          | 160673   | 4.767  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 95.400%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.031  | 65    |          | 73552    | 4.995  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 100.000% |          |
| 32) Benzene-d6                | 5.047  | 84    |          | 262636   | 3.891  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 77.800%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.069  | 67    |          | 95726    | 4.730  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 94.600%  |          |
| 41) Toluene-d8                | 7.317  | 98    |          | 182065   | 3.038  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 60.800%# |          |
| 43) trans-1,3-Dichloroprop... | 7.625  | 79    |          | 23849    | 3.601  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 72.000%  |          |
| 46) 2-Hexanone-d5             | 8.088  | 63    |          | 135379   | 47.219 | ug/L     | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 94.440%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.214 | 84    |          | 76775    | 4.869  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 97.400%  |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.622 | 152   |          | 77735    | 4.845  | ug/L     | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 96.800%  |          |
| Target Compounds              |        |       |          |          |        |          |          |
| 13) Acetone                   | 2.169  | 43    |          | 10916m   | 4.313  | ug/L     | Qvalue   |
| -----                         |        |       |          |          |        |          |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV072022\  
Data File : VV026847.D  
Acq On : 20 Jul 2022 12:18  
Operator : SY/MD  
Sample : N3754-15  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
GBHQ7

Manual IntegrationsAPPROVED

Quant Time: Jul 21 01:49:56 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR071122WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Jul 21 01:47:16 2022  
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/22/2022  
Supervised By :Semsettin Yesilyurt 07/22/2022

