

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
 Data File : VV026844.D
 Acq On : 20 Jul 2022 11:01
 Operator : SY/MD
 Sample : N3704-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jul 21 01:48:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 21 01:47:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	203989	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	216528	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	89795	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	97354	5.231	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.600%
7) Chloroethane-d5	1.561	69	87516	5.443	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.800%
11) 1,1-Dichloroethene-d2	2.101	63	139148	3.895	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.800%
20) 2-Butanone-d5	3.889	46	123630	42.565	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.140%
24) Chloroform-d	4.342	84	180016	5.532	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.600%
26) 1,2-Dichloroethane-d4	5.027	65	78472	5.520	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.400%
32) Benzene-d6	5.043	84	339111	5.154	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.000%
36) 1,2-Dichloropropane-d6	6.066	67	107159	5.432	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.600%
41) Toluene-d8	7.313	98	254919	4.365	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.200%
43) trans-1,3-Dichloroprop...	7.622	79	28917	4.480	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.600%
46) 2-Hexanone-d5	8.088	63	113628	40.662	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.320%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	74365	4.839	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.800%
66) 1,2-Dichlorobenzene-d4	11.622	152	87015	5.562	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.200%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	7655	0.359	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026844.D
Acq On : 20 Jul 2022 11:01
Operator : SY/MD
Sample : N3704-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jul 21 01:48:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 21 01:47:16 2022
Response via : Initial Calibration

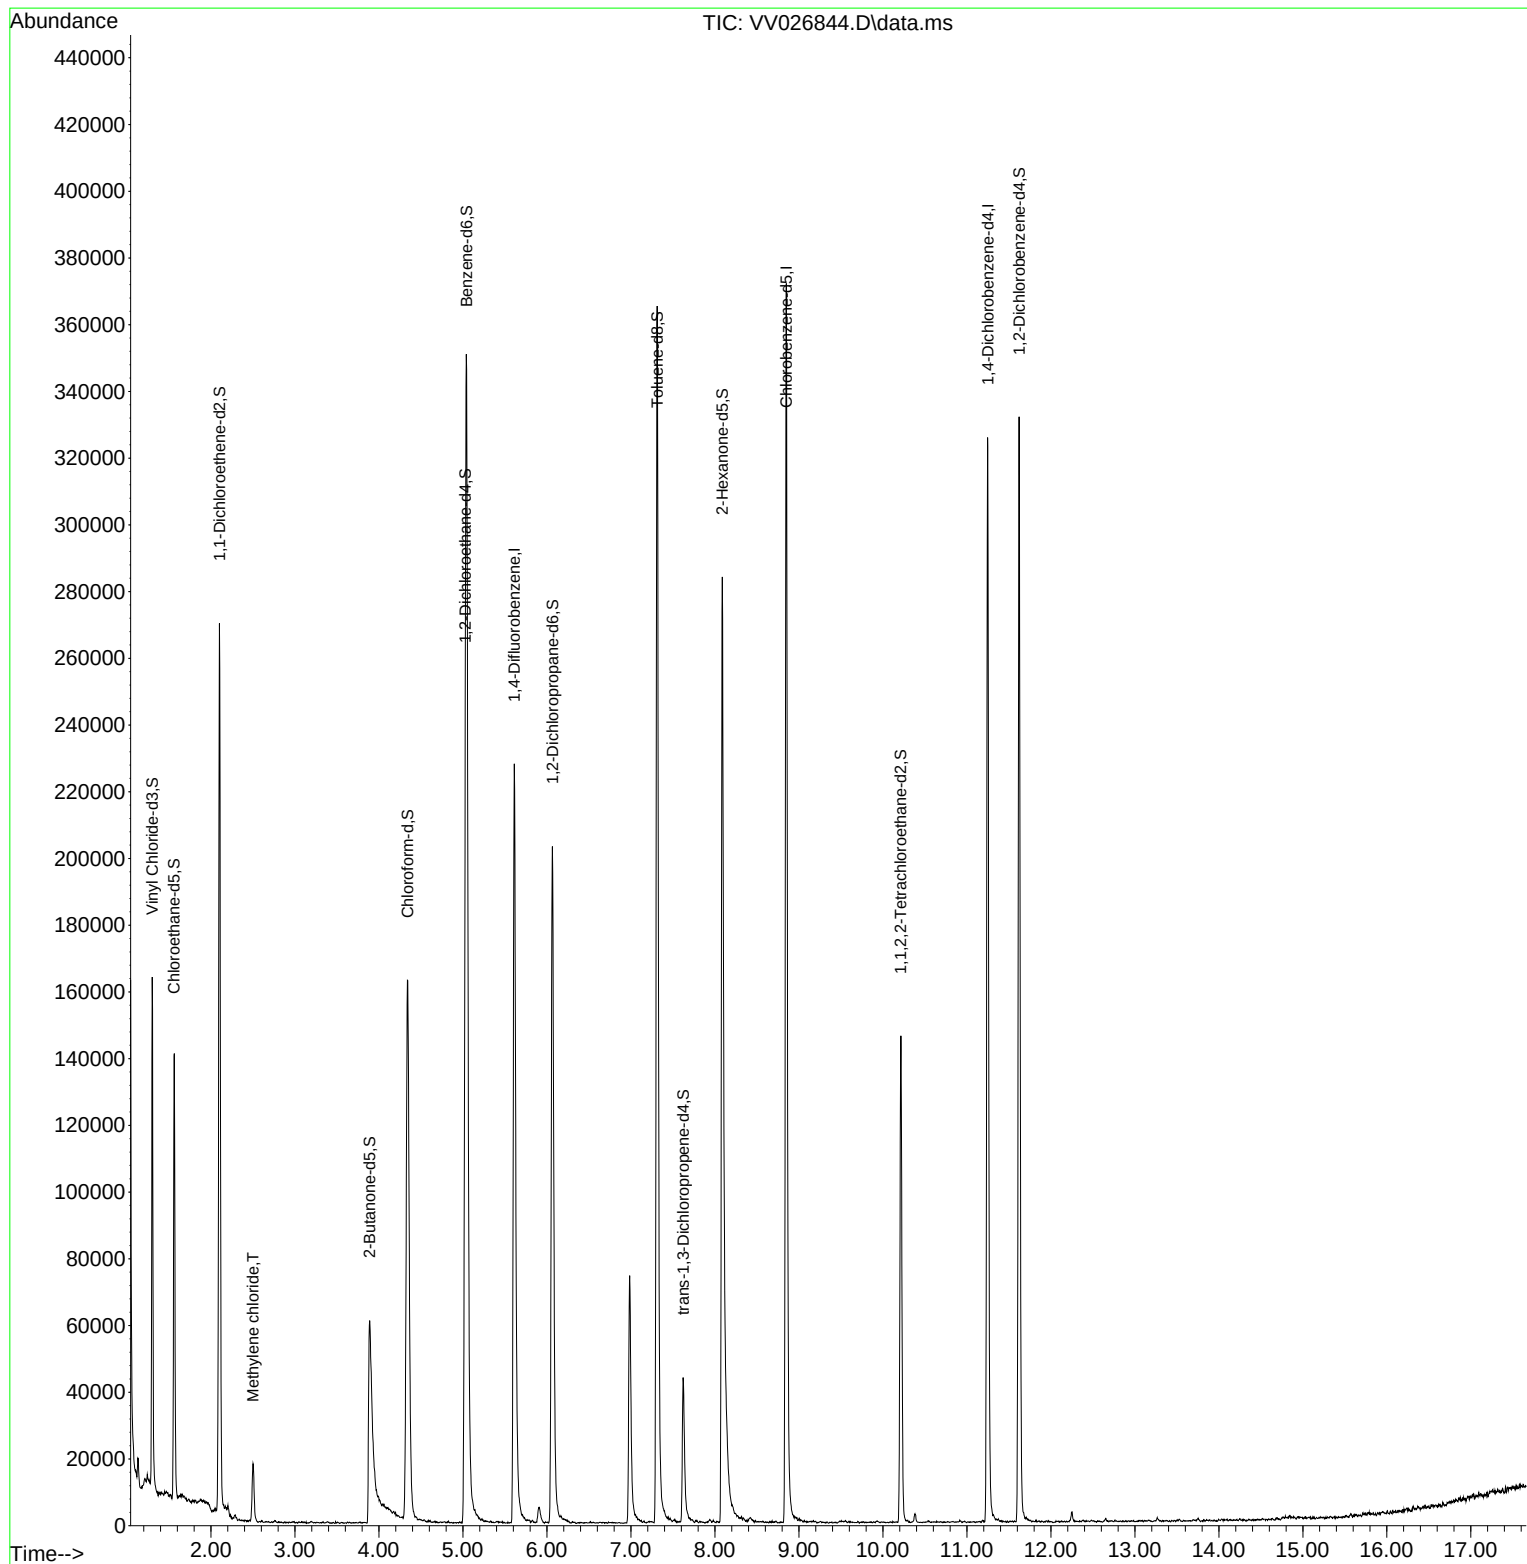

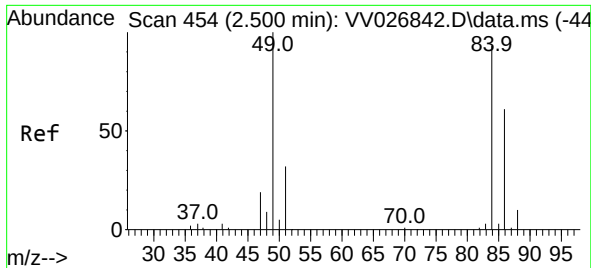

#16
Methylene chloride
Concen: 0.359 ug/L
RT: 2.500 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV026844.D
Acq: 20 Jul 2022 11:01

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

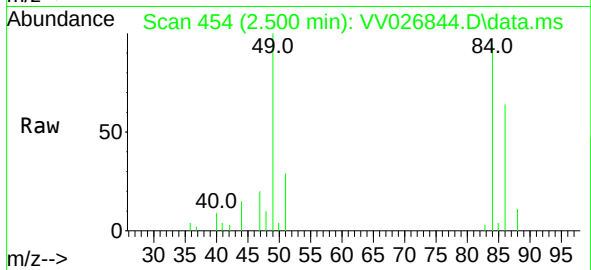

Tgt Ion: 84 Resp: 7655

Ion	Ratio	Lower	Upper
84	100		
86	67.9	44.8	83.2
49	106.0	78.7	146.1

