

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
 Data File : VV026847.D
 Acq On : 20 Jul 2022 12:18
 Operator : SY/MD
 Sample : N3754-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBHQ7

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/22/2022
 Supervised By :Semsettin Yesilyurt 07/22/2022

Quant Time: Jul 21 01:49:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 21 01:47:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	211288	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	222155	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	92090	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	64355	3.339	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	66.800%	
7) Chloroethane-d5	1.565	69	66119	3.970	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	79.400%	
11) 1,1-Dichloroethene-d2	2.102	63	88693	2.397	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	48.000%#	
20) 2-Butanone-d5	3.883	46	190050	63.173	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	126.340%	
24) Chloroform-d	4.346	84	160673	4.767	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.400%	
26) 1,2-Dichloroethane-d4	5.031	65	73552	4.995	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.000%	
32) Benzene-d6	5.047	84	262636	3.891	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	77.800%	
36) 1,2-Dichloropropane-d6	6.069	67	95726	4.730	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.600%	
41) Toluene-d8	7.317	98	182065	3.038	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	60.800%#	
43) trans-1,3-Dichloroprop...	7.625	79	23849	3.601	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	72.000%	
46) 2-Hexanone-d5	8.088	63	135379	47.219	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.440%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	76775	4.869	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	77735	4.845	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.800%	
Target Compounds					Qvalue	
13) Acetone	2.169	43	10916m	4.313	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026847.D
Acq On : 20 Jul 2022 12:18
Operator : SY/MD
Sample : N3754-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
GBHQ7

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/22/2022
Supervised By :Semsettin Yesilyurt 07/22/2022


Quant Time: Jul 21 01:49:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 21 01:47:16 2022
Response via : Initial Calibration

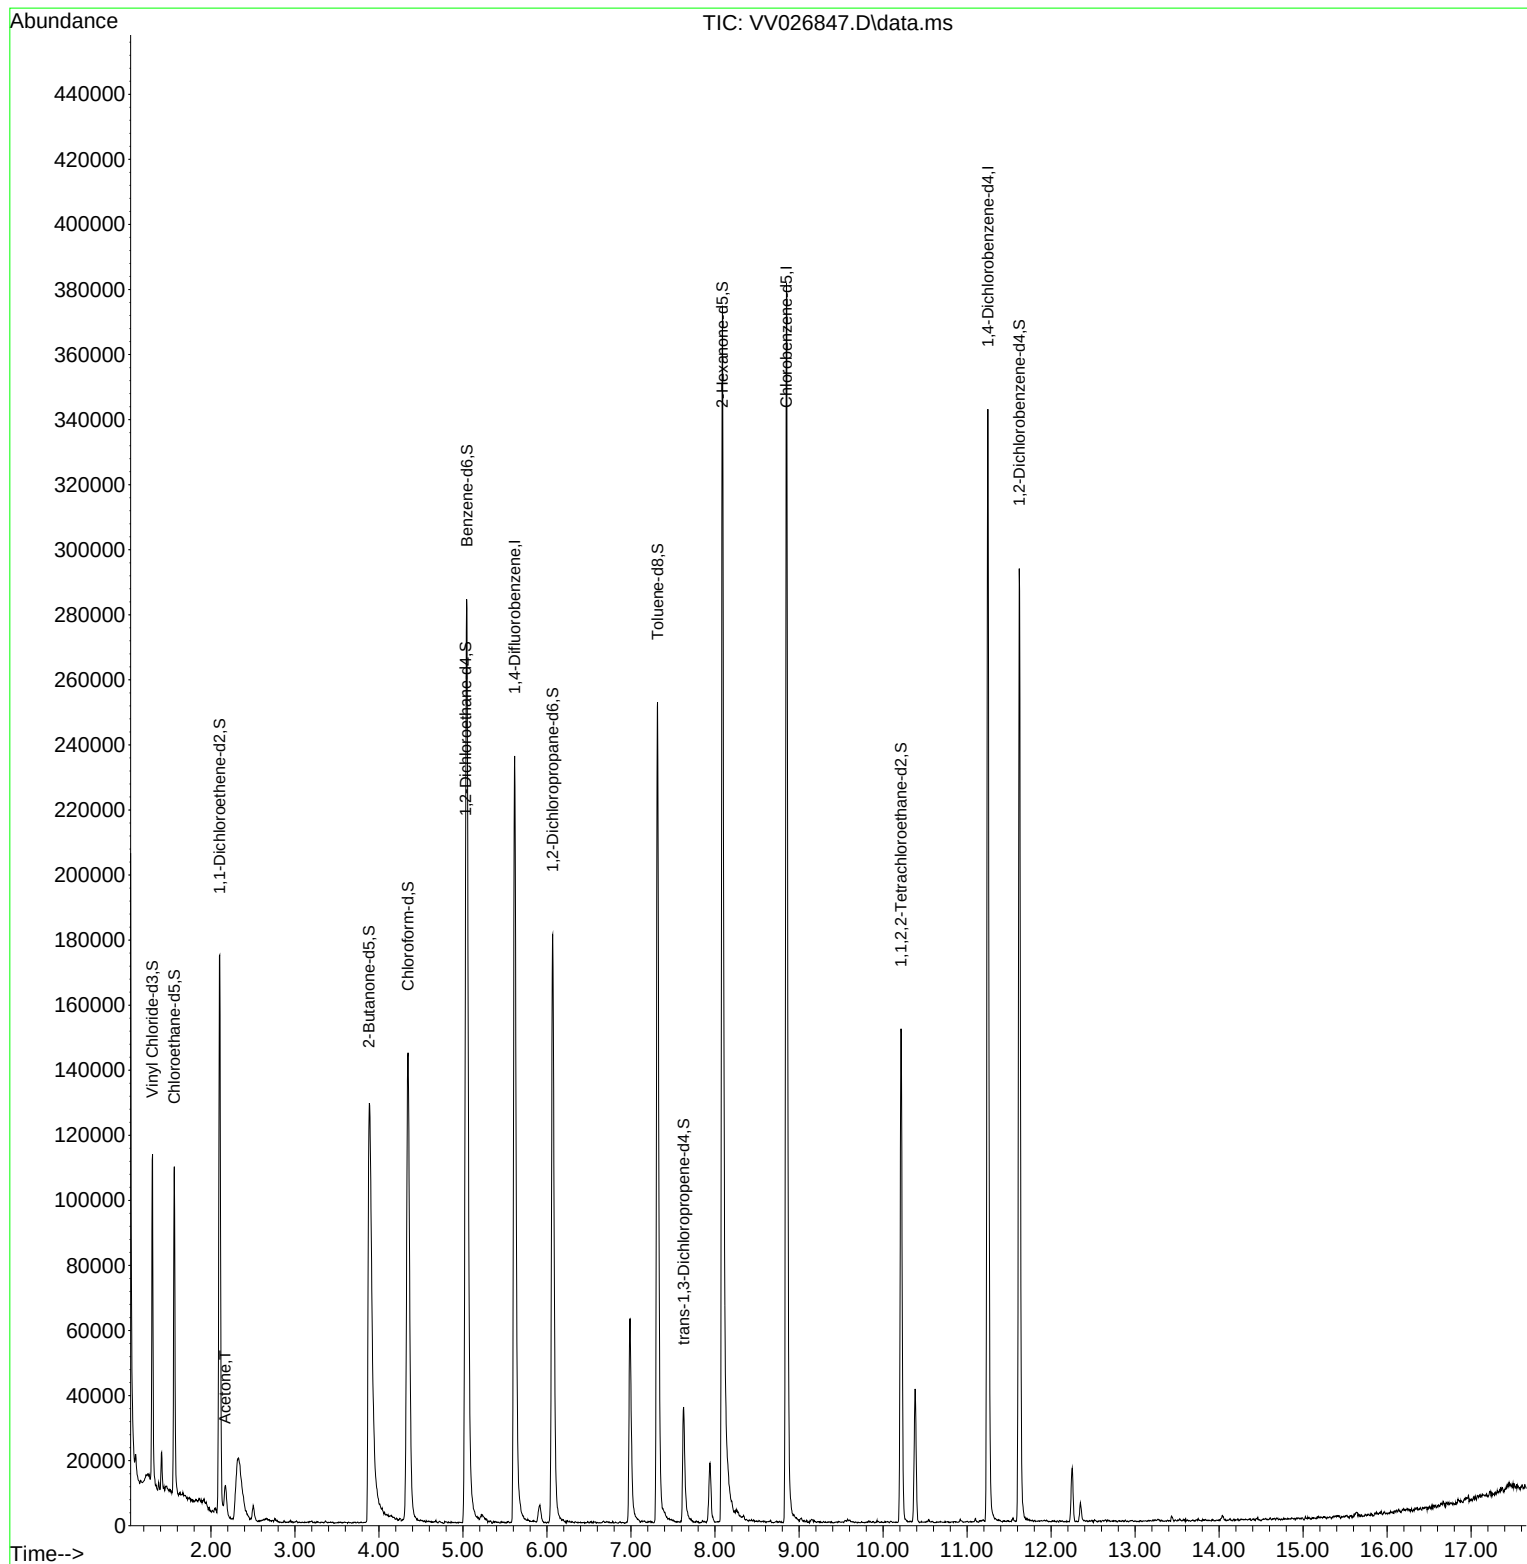

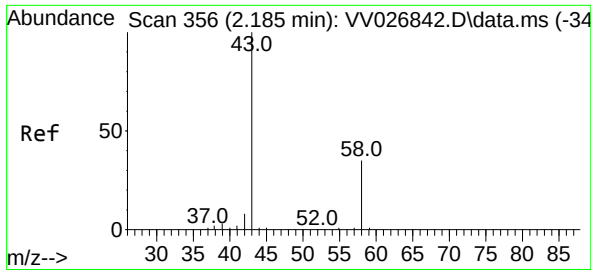

#13
Acetone
Concen: 4.313 ug/L m
RT: 2.169 min Scan# 3
Delta R.T. -0.016 min
Lab File: VV026847.D
Acq: 20 Jul 2022 12:18

Instrument :
MSVOA_V
ClientSampleId :
GBHQ7

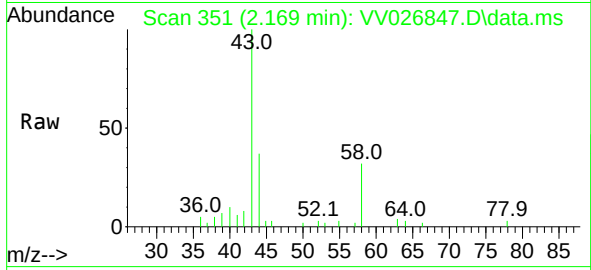

Tgt Ion: 43 Resp: 10910
Ion Ratio Lower Upper
43 100
58 7.3 0.0 20.6

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/22/2022
Supervised By :Semsettin Yesilyurt 07/22/2022

