

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
 Data File : VV026848.D
 Acq On : 20 Jul 2022 12:43
 Operator : SY/MD
 Sample : N3754-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jul 21 01:50:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jul 21 01:47:16 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.616	114	208392	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.850	117	215271	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.249	152	90359	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.301	65	95274	5.011	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	100.200%	
7) Chloroethane-d5		1.565	69	85757	5.221	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.400%	
11) 1,1-Dichloroethene-d2		2.101	63	136170	3.731	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.600%	
20) 2-Butanone-d5		3.883	46	152594	51.428	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.860%	
24) Chloroform-d		4.346	84	179836	5.410	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.200%	
26) 1,2-Dichloroethane-d4		5.031	65	78072	5.376	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.600%	
32) Benzene-d6		5.047	84	335340	5.126	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%	
36) 1,2-Dichloropropane-d6		6.069	67	104446	5.325	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.600%	
41) Toluene-d8		7.313	98	252105	4.342	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.800%	
43) trans-1,3-Dichloroprop...		7.625	79	28989	4.518	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5		8.088	63	114836	41.335	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.660%	
56) 1,1,2,2-Tetrachloroeth...		10.217	84	75898	4.968	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.400%	
66) 1,2-Dichlorobenzene-d4		11.622	152	87801	5.577	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.600%	
Target Compounds						Qvalue	
16) Methylene chloride		2.503	84	4782	0.220	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026848.D
Acq On : 20 Jul 2022 12:43
Operator : SY/MD
Sample : N3754-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Jul 21 01:50:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jul 21 01:47:16 2022
Response via : Initial Calibration

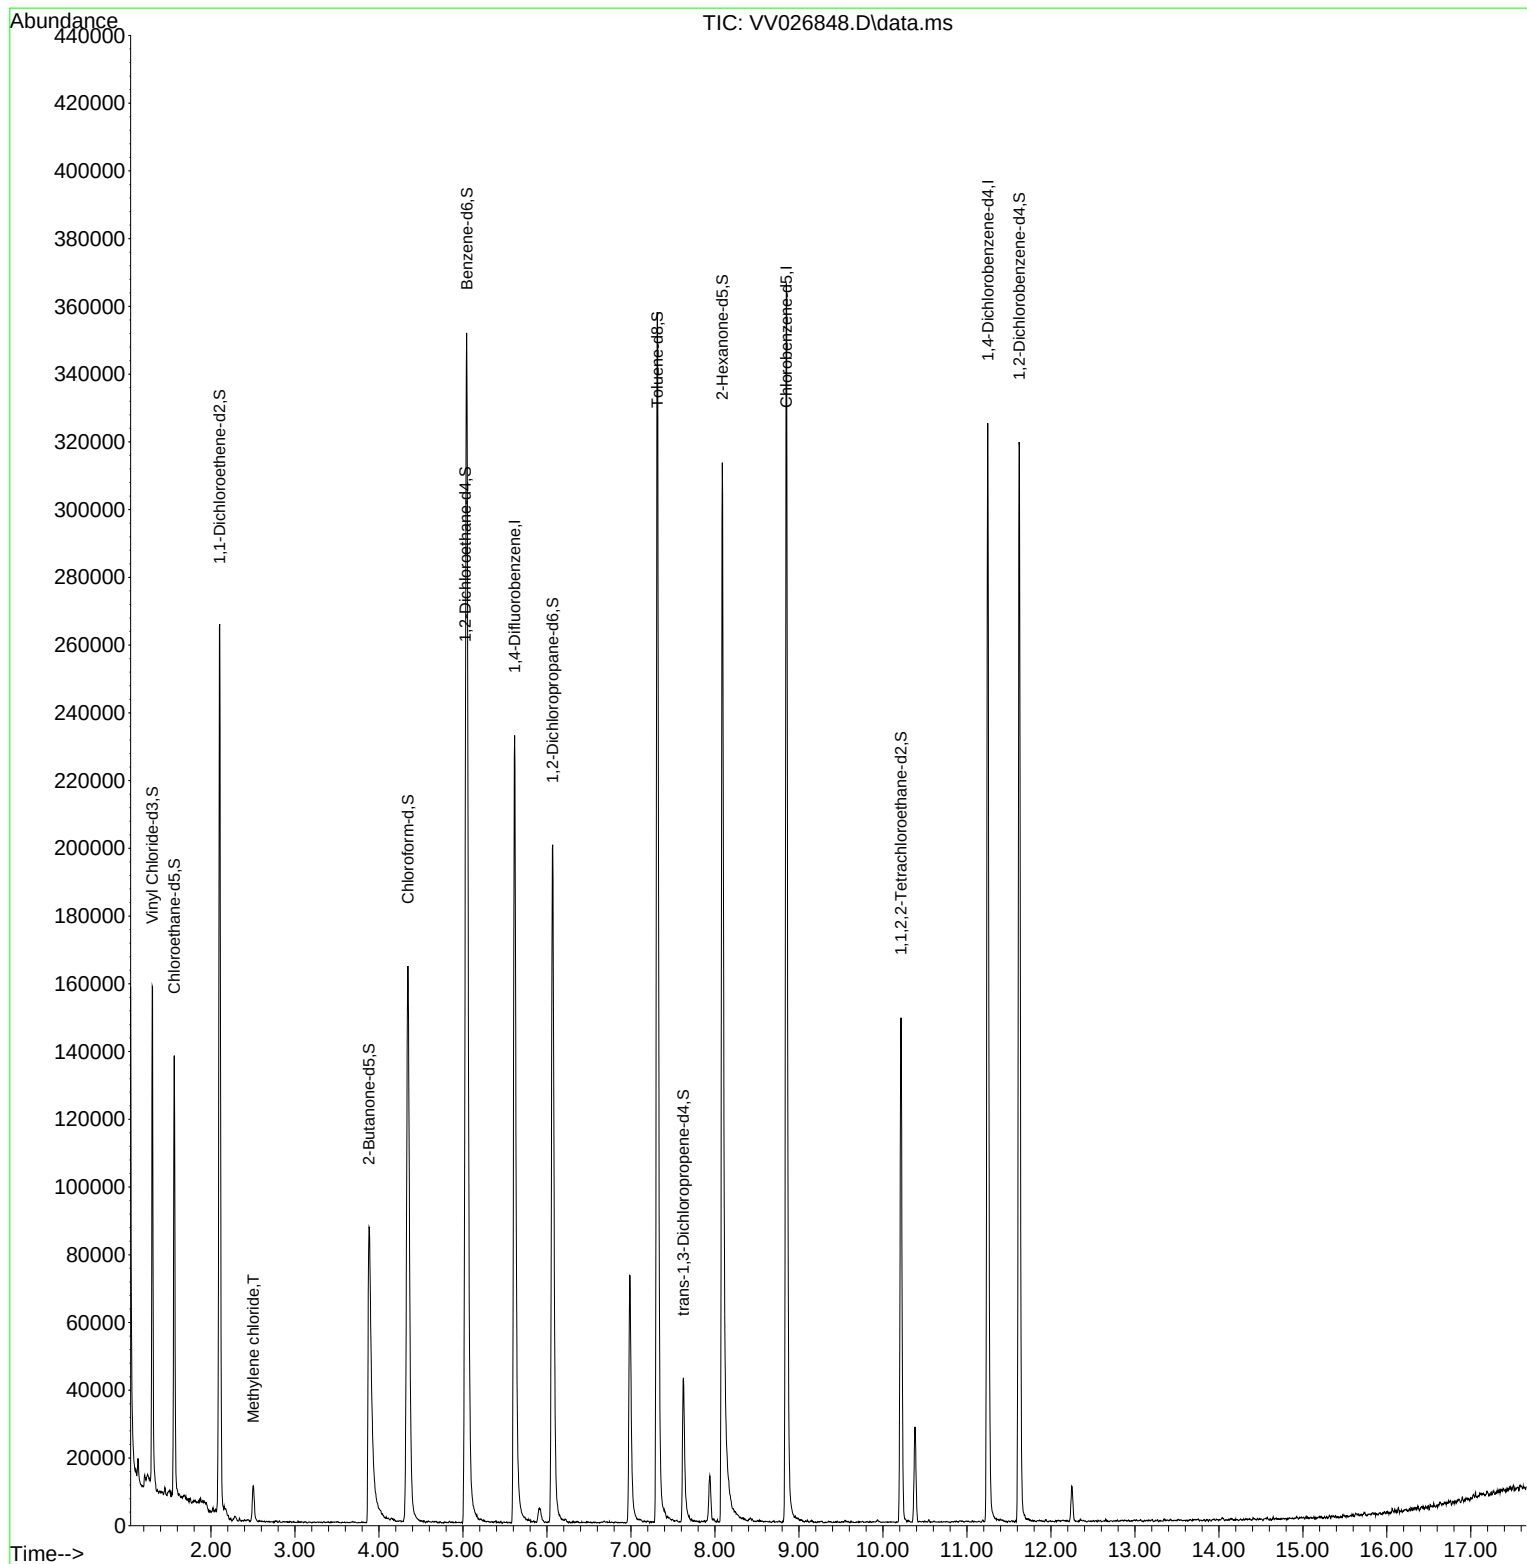

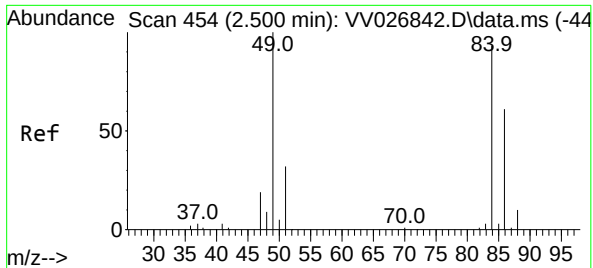

#16
Methylene chloride
Concen: 0.220 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV026848.D
Acq: 20 Jul 2022 12:43

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 4782

Ion	Ratio	Lower	Upper
84	100		
86	63.6	44.8	83.2
49	108.3	78.7	146.1

