

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
 Data File : VV026843.D
 Acq On : 20 Jul 2022 10:25
 Operator : SY/MD
 Sample : VV0720WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK398

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026843.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	25	29	39	rVB	11550	14295	1.51%	0.201%
2	1.304	75	82	95	rVB	164556	166801	17.63%	2.349%
3	1.565	155	163	180	rVB	147208	169006	17.87%	2.380%
4	1.905	265	269	273	rVB	19375	10770	1.14%	0.152%
5	2.105	320	331	350	rBV	285665	408539	43.19%	5.753%
6	2.503	444	455	468	rVB	16805	27884	2.95%	0.393%
7	3.899	877	889	925	rBV2	77149	283996	30.02%	3.999%
8	4.346	1010	1028	1053	rBV	177671	446927	47.25%	6.293%
9	5.043	1229	1245	1272	rBV2	376196	945904	100.00%	13.319%
10	5.616	1410	1423	1456	rBV	239284	504658	53.35%	7.106%
11	5.915	1504	1516	1529	rVB9	4920	11498	1.22%	0.162%
12	6.069	1551	1564	1586	rBV	220452	461346	48.77%	6.496%
13	6.986	1839	1849	1868	rBV	79162	154596	16.34%	2.177%
14	7.313	1938	1951	1972	rBV	391388	699190	73.92%	9.845%
15	7.625	2034	2048	2071	rBV	49300	93152	9.85%	1.312%
16	8.088	2182	2192	2225	rBV	343338	687111	72.64%	9.675%
17	8.850	2413	2429	2460	rBV	389965	656554	69.41%	9.245%
18	10.214	2841	2853	2870	rBV	163282	258688	27.35%	3.643%
19	11.246	3164	3174	3196	rBV	341738	542679	57.37%	7.642%
20	11.622	3277	3291	3309	rBV	353596	558110	59.00%	7.859%




Sum of corrected areas: 7101704

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026843.D
Acq On : 20 Jul 2022 10:25
Operator : SY/MD
Sample : VV0720WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK398

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

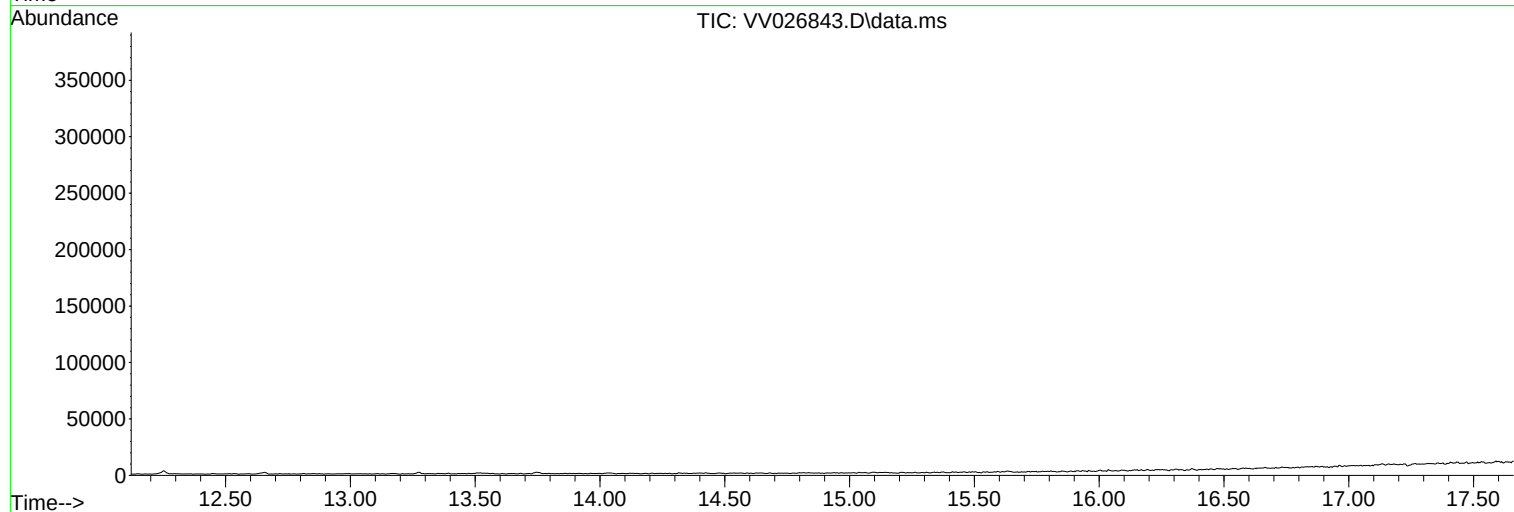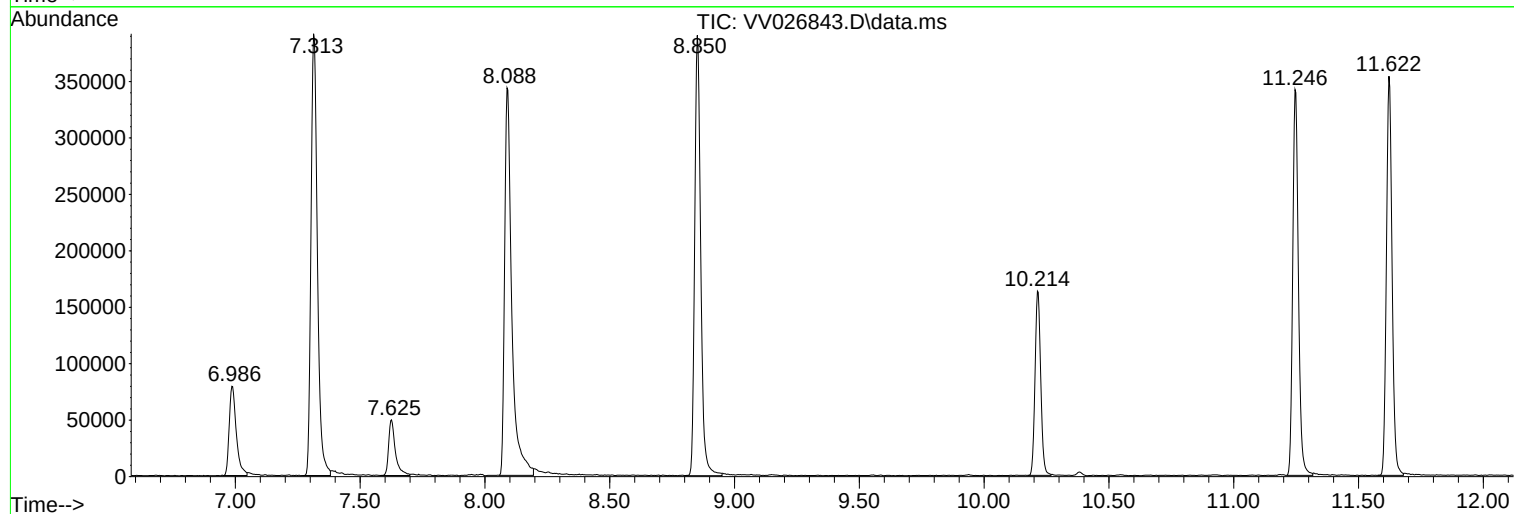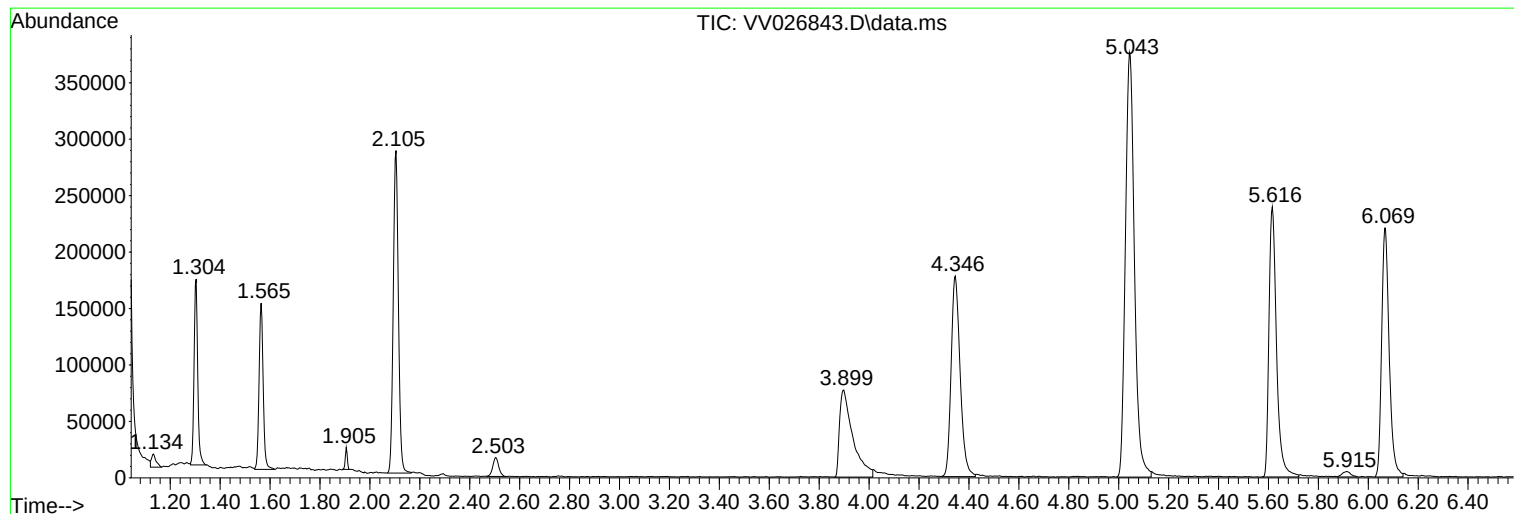

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026843.D
Acq On : 20 Jul 2022 10:25
Operator : SY/MD
Sample : VV0720WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK398

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026843.D
Acq On : 20 Jul 2022 10:25
Operator : SY/MD
Sample : VV0720WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK398

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc