

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
 Data File : VV026848.D
 Acq On : 20 Jul 2022 12:43
 Operator : SY/MD
 Sample : N3754-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026848.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	149024	158438	18.06%	2.381%
2	1.565	155	163	178	rVB	129790	150397	17.15%	2.260%
3	2.105	319	331	346	rBV	261996	373943	42.63%	5.620%
4	2.503	444	455	473	rVB2	10687	18970	2.16%	0.285%
5	3.883	874	884	925	rBV	87371	267483	30.49%	4.020%
6	4.346	1011	1028	1068	rBV	163991	411280	46.89%	6.181%
7	5.043	1230	1245	1282	rBV2	351446	877157	100.00%	13.182%
8	5.616	1410	1423	1458	rBV	232567	483042	55.07%	7.259%
9	6.069	1550	1564	1588	rBV	200071	424087	48.35%	6.373%
10	6.986	1835	1849	1880	rBV	73226	145755	16.62%	2.190%
11	7.313	1940	1951	1977	rBV	357337	648698	73.95%	9.749%
12	7.625	2038	2048	2069	rBV2	42549	81392	9.28%	1.223%
13	7.940	2134	2146	2156	rBV2	13291	22949	2.62%	0.345%
14	8.088	2182	2192	2232	rBV	312781	632906	72.15%	9.512%
15	8.850	2417	2429	2459	rBV	365606	615133	70.13%	9.244%
16	10.217	2842	2854	2868	rBV	148932	237238	27.05%	3.565%
17	10.381	2895	2905	2917	rBV3	28191	45689	5.21%	0.687%
18	11.249	3163	3175	3202	rBV	324364	521826	59.49%	7.842%
19	11.622	3280	3291	3310	rBV	318849	520770	59.37%	7.826%
20	12.249	3476	3486	3499	rBV2	10452	16928	1.93%	0.254%




Sum of corrected areas: 6654081

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026848.D
Acq On : 20 Jul 2022 12:43
Operator : SY/MD
Sample : N3754-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

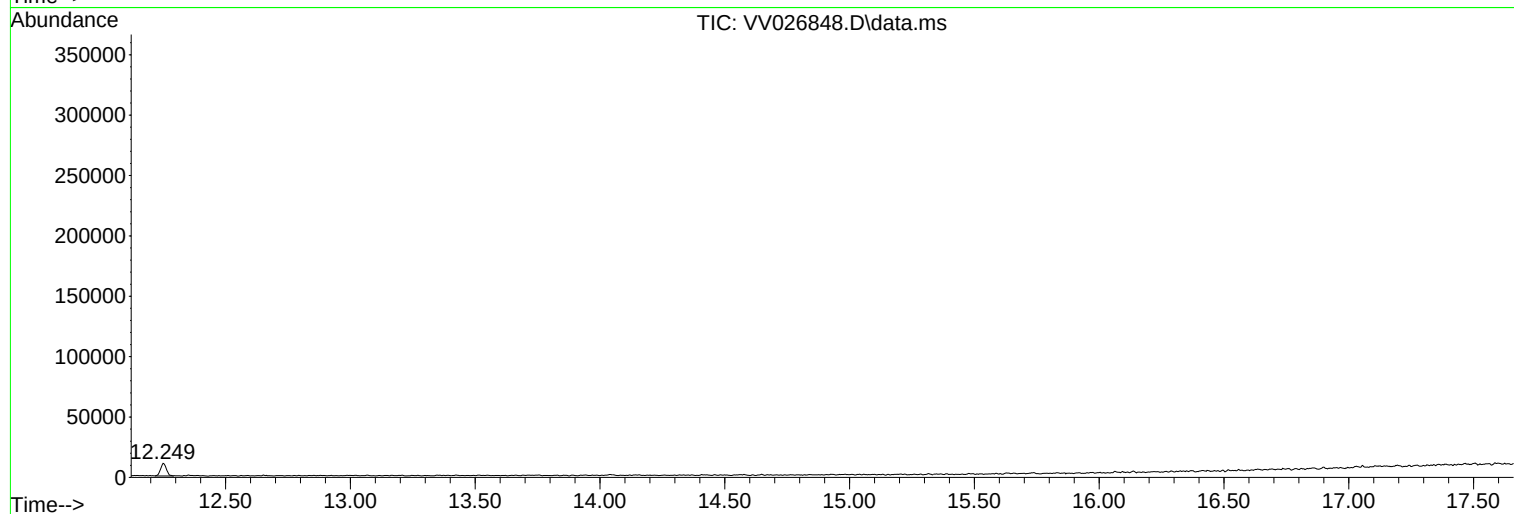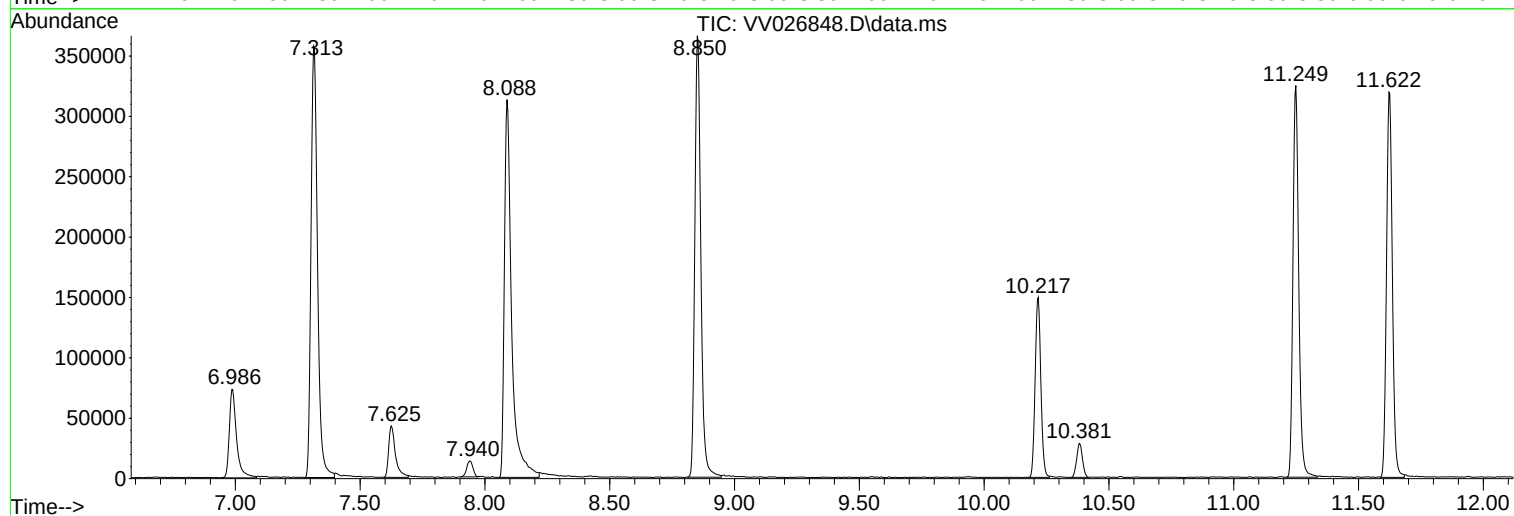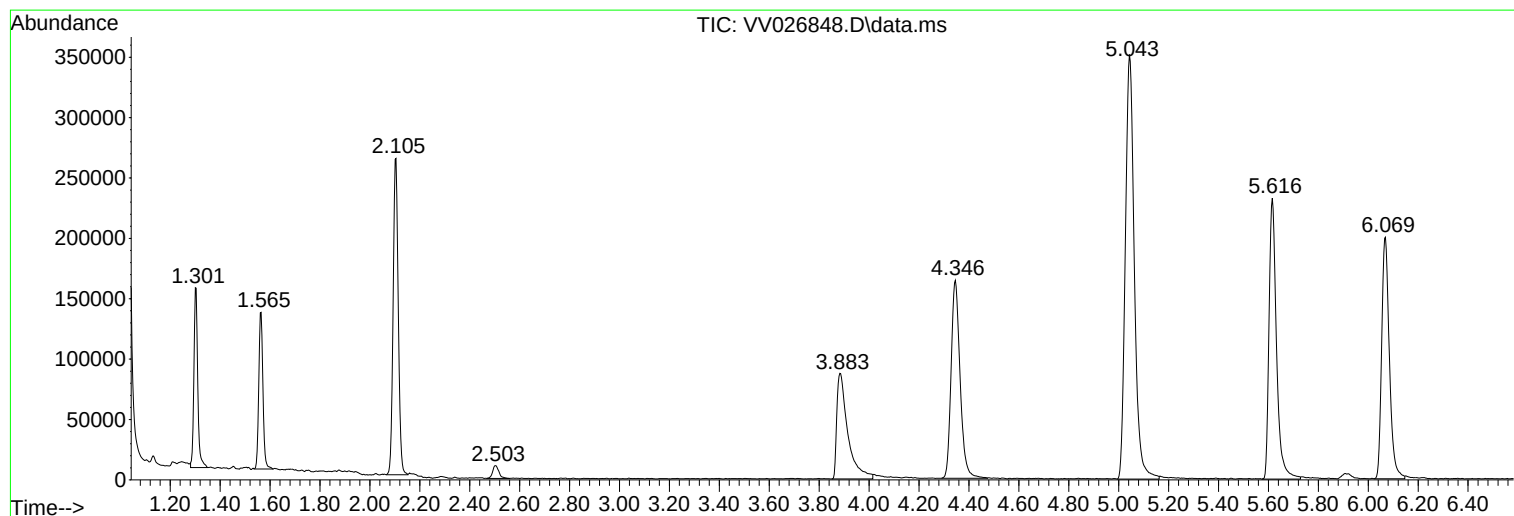

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026848.D
Acq On : 20 Jul 2022 12:43
Operator : SY/MD
Sample : N3754-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
Data File : VV026848.D
Acq On : 20 Jul 2022 12:43
Operator : SY/MD
Sample : N3754-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc