
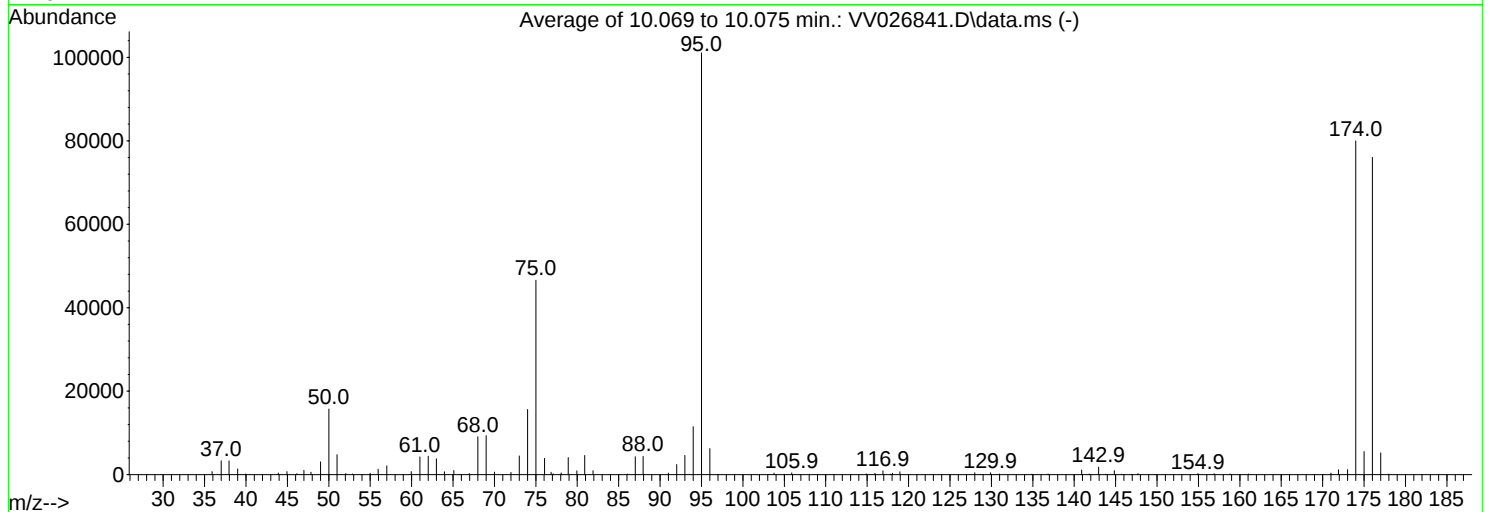


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072022\
 Data File : VV026841.D
 Acq On : 20 Jul 2022 08:56
 Operator : SY/MD
 Sample : BFB349
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB349

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR071122WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Jul 21 01:47:16 2022

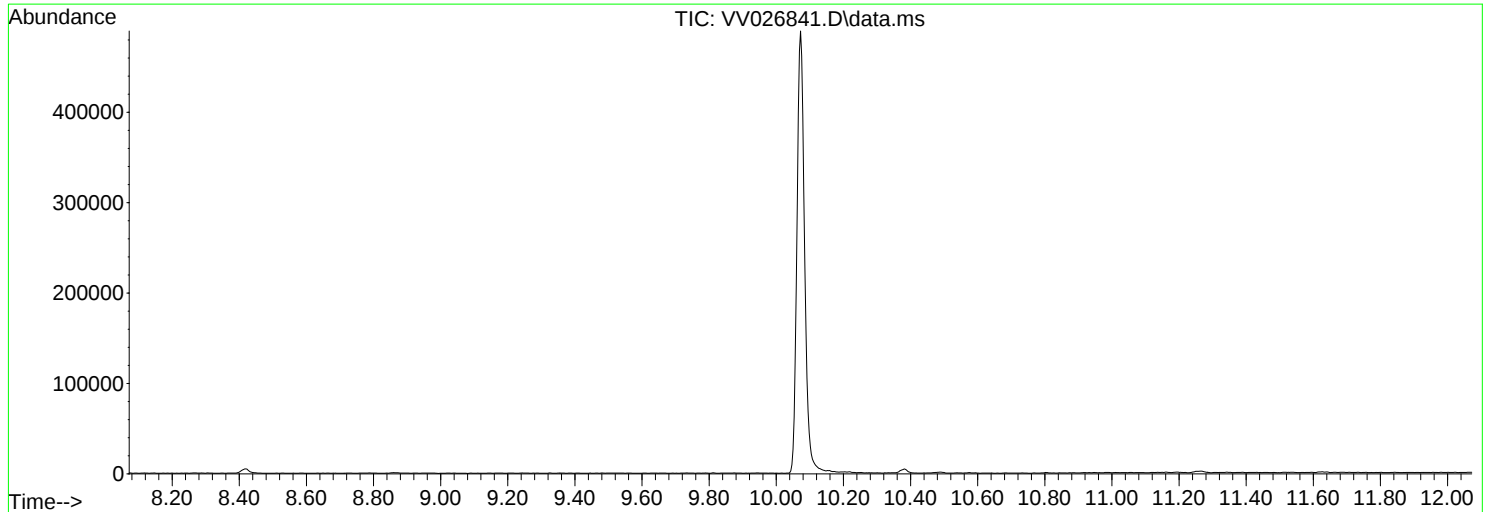

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	15741	PASS
75	95	30	80	46.1	46611	PASS
95	95	100	100	100.0	101083	PASS
96	95	5	9	6.2	6240	PASS
173	174	0.00	2	1.5	1199	PASS
174	95	50	120	79.1	79968	PASS
175	174	5	9	6.9	5530	PASS
176	174	95	105	95.1	76029	PASS
177	176	5	10	6.9	5227	PASS

m/z	Abundance
39.90	337.0
43.90	495.0

Instrument :
MSVOA_V
ClientSampleId :
BFB349

m/z	Abundance
35.90	760.0
37.00	3464.0
38.00	3474.0
39.00	1406.0
40.10	496.0
43.90	910.0
44.90	728.0
46.20	220.0
47.00	1003.0
47.90	574.0
49.00	3183.0
50.00	16056.0
51.00	4842.0
52.00	257.0
52.80	173.0
55.00	330.0
55.90	1214.0
57.00	2113.0
59.90	855.0
61.00	4438.0
62.00	4616.0
63.00	3688.0
63.90	706.0
65.10	1058.0
65.80	101.0
67.00	289.0
68.00	9192.0
69.00	9503.0
70.00	663.0
72.00	536.0
73.00	4614.0
74.00	15582.0
75.00	46376.0
76.10	4139.0
76.90	561.0
77.10	545.0
78.00	516.0
78.90	4017.0
79.90	966.0
80.90	4478.0
81.90	946.0
86.10	107.0
87.00	4411.0
87.90	4547.0
91.00	357.0
92.00	2460.0
93.00	4412.0
94.00	11404.0
95.00	99712.0
96.00	6163.0
97.00	200.0
103.70	389.0
105.90	426.0
108.10	117.0
110.90	105.0
114.90	171.0
116.00	332.0
116.90	867.0
118.00	356.0
119.00	693.0
128.00	410.0
128.70	136.0
129.90	444.0
131.00	154.0
134.80	128.0
136.80	148.0
140.90	1031.0
141.80	150.0
142.90	1790.0
144.80	915.0
146.10	126.0
146.90	102.0
147.70	210.0
154.90	257.0
157.00	273.0
158.80	162.0
161.00	209.0
171.00	401.0
171.90	992.0
173.00	1131.0
174.00	77448.0
175.00	5290.0
176.00	73368.0
177.00	5092.0
178.00	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB349

m/z	Abundance
35.90	756.0
37.00	3443.0
37.90	3434.0
39.00	1413.0
40.10	479.0
44.00	916.0
45.00	752.0
46.10	211.0
47.00	1103.0
47.90	615.0
49.00	3146.0
50.00	16243.0
51.00	4913.0
52.00	277.0
52.80	173.0
55.00	364.0
56.00	1329.0
57.00	2207.0
59.90	751.0
61.00	4388.0
62.00	4586.0
63.00	3930.0
64.00	680.0
65.10	1061.0
67.00	288.0
68.00	9423.0
69.00	9631.0
70.00	664.0
72.00	542.0
73.00	4679.0
74.00	16136.0
75.00	48224.0
76.00	3994.0
76.80	582.0
78.00	432.0
78.90	4174.0
79.90	962.0
80.90	4811.0
81.90	1023.0
86.00	145.0
87.00	4424.0
87.90	4532.0
91.00	397.0
92.00	2476.0
93.00	4804.0
94.00	11886.0
95.00	105280.0
96.00	6390.0
103.70	407.0
105.00	108.0
105.90	405.0
106.90	122.0
108.10	106.0
110.90	121.0
114.90	212.0
116.00	333.0
116.90	951.0
118.10	398.0
118.90	709.0
128.00	475.0
128.70	154.0
129.90	482.0
131.00	172.0
134.90	131.0
136.90	143.0
140.90	1148.0
141.80	158.0
143.00	1896.0
143.80	178.0
144.80	979.0
145.70	155.0
147.70	265.0
155.00	283.0
156.90	247.0
158.80	181.0
161.00	180.0
171.00	426.0
171.90	1209.0
173.00	1244.0
174.00	82688.0
175.00	5703.0
176.00	78784.0
177.00	5440.0
178.00	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB349

m/z	Abundance
35.90	644.0
37.00	3061.0
37.90	3010.0
39.00	1323.0
39.90	493.0
44.00	832.0
45.00	724.0
46.10	216.0
47.00	961.0
47.80	587.0
49.00	2832.0
50.00	14923.0
51.00	4607.0
52.10	299.0
52.90	176.0
54.00	131.0
55.00	290.0
56.00	1340.0
57.00	2052.0
60.00	614.0
61.00	3927.0
62.00	4033.0
63.00	3796.0
64.00	680.0
65.10	935.0
66.90	282.0
68.00	8645.0
69.00	8900.0
70.00	556.0
72.00	502.0
73.00	4136.0
74.00	15087.0
75.00	45232.0
76.00	3620.0
76.80	586.0
78.10	357.0
78.90	4098.0
80.00	869.0
80.90	4509.0
81.90	952.0
86.00	198.0
87.00	4095.0
88.00	4052.0
91.00	420.0
92.00	2355.0
93.00	4623.0
94.00	11191.0
95.00	98256.0
96.00	6166.0
103.80	376.0
104.90	129.0
105.90	380.0
106.90	155.0
107.90	103.0
114.90	223.0
115.90	282.0
116.90	921.0
117.80	348.0
118.10	321.0
118.90	670.0
128.00	453.0
129.00	171.0
129.90	428.0
131.00	169.0
135.00	113.0
136.90	120.0
140.90	1109.0
141.80	144.0
143.00	1704.0
143.80	159.0
144.90	941.0
145.80	168.0
147.70	294.0
149.70	121.0
155.00	279.0
156.80	193.0
158.80	179.0
161.10	130.0
171.00	361.0
171.90	1276.0
173.00	1221.0
174.00	79768.0
175.00	5596.0
176.00	75936.0
177.00	5148.0
178.00	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB349