


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV072023\
Data File : VV031723.D
Acq On : 20 Jul 2023 10:02
Operator : SY/MD
Sample : BFB242
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB242

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM071923.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jul 20 05:08:22 2023

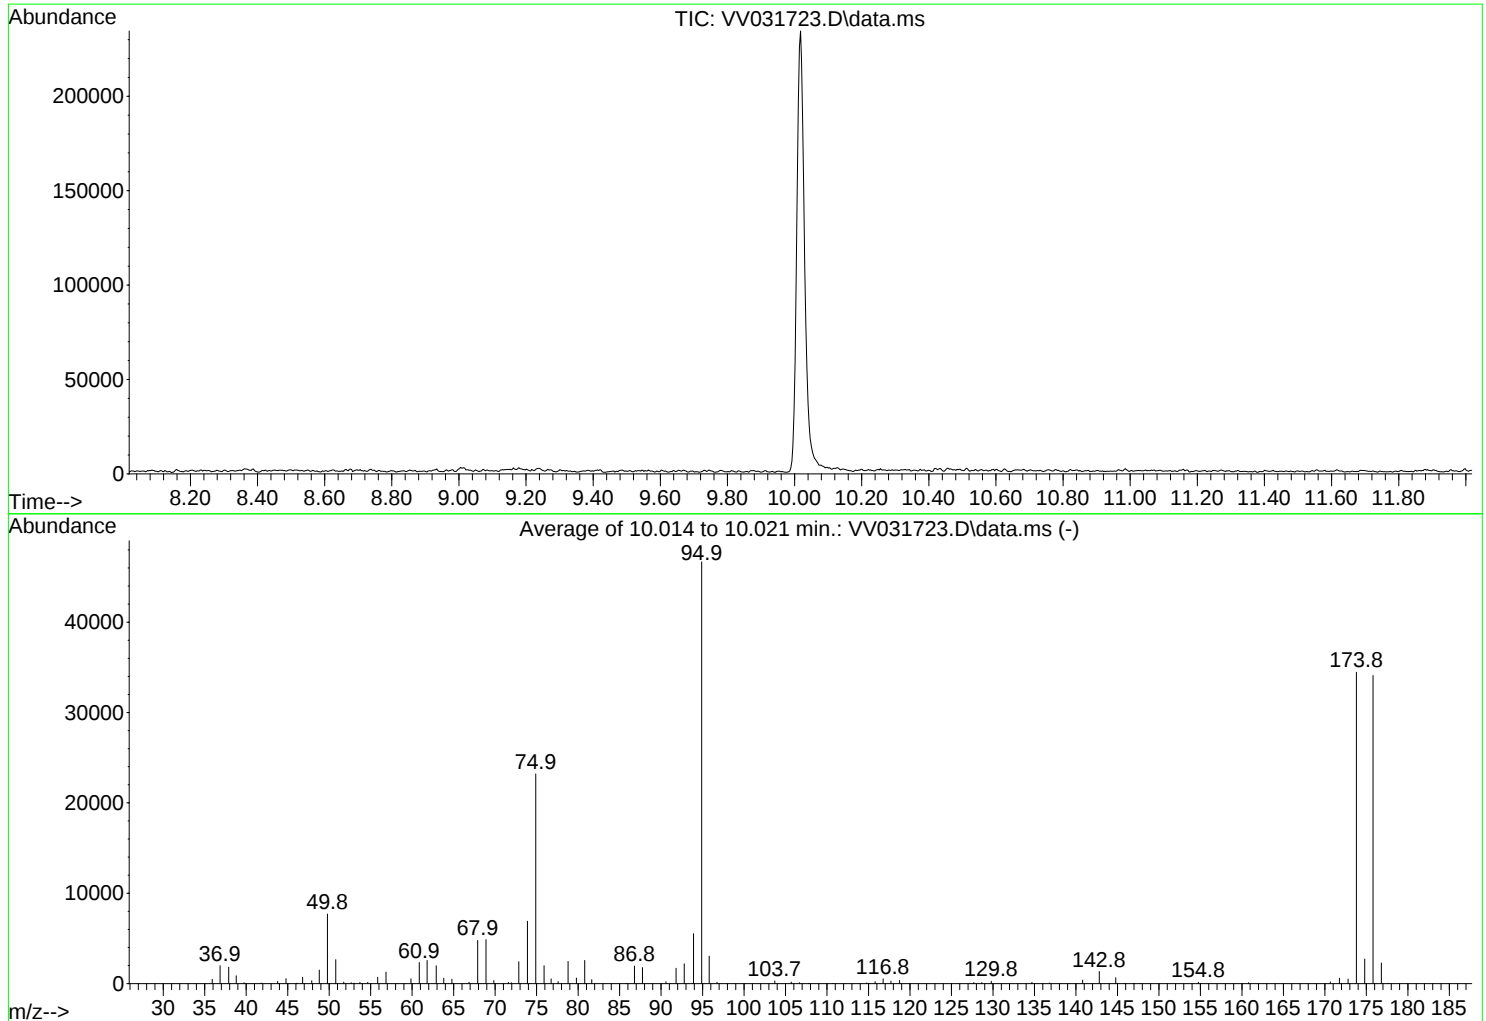

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	7695	PASS
75	95	30	80	49.7	23216	PASS
95	95	100	100	100.0	46675	PASS
96	95	5	9	6.5	3041	PASS
173	174	0.00	2	1.5	510	PASS
174	95	50	120	73.8	34451	PASS
175	174	5	9	7.9	2737	PASS
176	174	95	101	99.0	34096	PASS
177	176	5	9	6.7	2286	PASS

m/z	Abundance
39.80	315.0
43.80	534.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
35.90	445.0
36.90	1906.0
37.90	1884.0
38.80	1000.0
39.80	329.0
43.80	735.0
44.80	630.0
46.10	143.0
46.80	651.0
47.90	264.0
48.80	1625.0
49.80	7841.0
50.80	2694.0
51.80	104.0
52.60	176.0
53.70	157.0
54.60	126.0
55.90	633.0
56.90	1255.0
59.80	518.0
60.80	2097.0
61.80	2712.0
62.90	2187.0
63.80	610.0
64.80	477.0
66.80	183.0
67.90	4830.0
68.90	4941.0
69.80	355.0
71.60	133.0
72.80	2469.0
73.90	6966.0
74.90	23784.0
75.90	2194.0
76.80	519.0
77.60	265.0
78.80	2444.0
79.80	611.0
80.80	2515.0
81.60	373.0
85.80	110.0
86.80	1975.0
87.80	1666.0
90.60	217.0
91.80	1777.0
92.80	2203.0
93.90	5538.0
94.90	46656.0
95.80	3232.0
96.80	173.0
103.70	311.0
105.70	231.0
106.70	163.0
115.80	272.0
116.70	534.0
117.70	273.0
118.70	363.0
128.60	113.0
129.80	230.0
134.70	144.0
140.80	375.0
142.80	1309.0
144.80	506.0
147.70	115.0
154.80	179.0
170.70	245.0
171.80	606.0
172.80	763.0
173.80	33776.0
174.80	2910.0
175.80	33200.0
176.80	2206.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
35.90	516.0
36.90	2099.0
37.90	1901.0
38.80	883.0
39.70	447.0
41.80	107.0
43.80	784.0
44.80	561.0
46.80	727.0
47.90	363.0
48.80	1556.0
49.80	7962.0
50.80	2740.0
51.70	181.0
52.70	140.0
53.70	157.0
54.70	136.0
55.80	708.0
56.80	1315.0
59.90	560.0
60.90	2439.0
61.80	2668.0
62.90	2046.0
63.80	642.0
64.80	520.0
66.90	148.0
67.90	5071.0
68.90	4969.0
69.90	339.0
71.60	139.0
71.90	136.0
72.80	2509.0
73.90	7055.0
74.90	24024.0
75.90	2026.0
76.80	560.0
77.60	252.0
78.80	2554.0
79.80	675.0
80.80	2675.0
81.60	457.0
86.80	1993.0
87.80	1889.0
90.60	226.0
91.80	1777.0
92.80	2280.0
93.90	5668.0
94.90	48328.0
95.80	3123.0
96.70	157.0
103.70	319.0
105.70	174.0
106.70	136.0
110.70	109.0
114.80	128.0
115.80	225.0
116.70	580.0
117.70	309.0
118.70	358.0
127.70	165.0
128.70	128.0
129.80	261.0
134.70	144.0
136.80	108.0
140.80	411.0
142.80	1389.0
144.80	707.0
147.00	120.0
154.80	160.0
160.80	137.0
170.70	181.0
171.80	583.0
172.80	768.0
173.80	35464.0
174.80	2832.0
175.80	35160.0
176.80	2340.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242

m/z	Abundance
35.90	470.0
36.80	1962.0
37.90	1691.0
38.80	738.0
39.70	513.0
41.80	137.0
43.90	838.0
44.80	458.0
46.80	746.0
47.90	359.0
48.80	1337.0
49.80	7283.0
50.80	2518.0
51.70	230.0
53.00	152.0
53.70	118.0
54.70	139.0
55.80	778.0
56.80	1235.0
59.90	493.0
60.90	2503.0
61.80	2308.0
62.90	1694.0
63.80	564.0
64.80	515.0
66.90	151.0
67.90	4452.0
68.90	4707.0
69.90	323.0
71.60	140.0
72.00	202.0
72.90	2283.0
73.90	6710.0
74.90	21840.0
75.90	1754.0
76.70	528.0
77.60	198.0
78.80	2371.0
79.80	557.0
80.80	2513.0
81.70	478.0
86.80	1893.0
87.70	1748.0
90.60	213.0
91.80	1539.0
92.80	2094.0
93.90	5385.0
94.90	45040.0
95.80	2768.0
96.70	135.0
103.70	254.0
105.70	118.0
107.80	114.0
114.80	162.0
115.80	178.0
116.80	502.0
117.70	290.0
118.80	320.0
127.70	215.0
128.70	112.0
129.80	285.0
134.70	128.0
136.80	107.0
140.80	392.0
142.80	1325.0
144.80	770.0
145.80	111.0
154.70	134.0
160.80	167.0
170.60	147.0
171.70	605.0
173.80	34112.0
174.80	2470.0
175.80	33928.0
176.80	2312.0
177.70	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB242