

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072118\
 Data File : VV006680.D
 Acq On : 21 Jul 2018 12:20
 Operator : SY/MD
 Sample : J4078-06
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0

Quant Time: Jul 22 23:11:30 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jul 22 23:06:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	227883	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	209354	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	83595	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	83268	5.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	104.20%
7) Chloroethane-d5	1.58	69	64783	6.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	120.00%
11) 1,1-Dichloroethene-d2	2.13	63	119622	3.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.80%
20) 2-Butanone-d5	3.95	46	174882	50.35	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.70%
24) Chloroform-d	4.40	84	144364	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.20%
26) 1,2-Dichloroethane-d4	5.09	65	70231	5.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.60%
32) Benzene-d6	5.10	84	313967	5.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.40%
36) 1,2-Dichloropropane-d6	6.12	67	96290	5.46	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	109.20%
41) Toluene-d8	7.36	98	264272	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.00%
43) trans-1,3-Dichloropropene-	7.67	79	24300	4.06	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.20%
46) 2-Hexanone-d5	8.14	63	138249	46.35	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.70%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	63114	4.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	88267	5.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	9463	3.55 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072118\
Data File : VV006680.D
Acq On : 21 Jul 2018 12:20
Operator : SY/MD
Sample : J4078-06
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Quant Time: Jul 22 23:11:30 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jul 22 23:06:02 2018
Response via : Initial Calibration

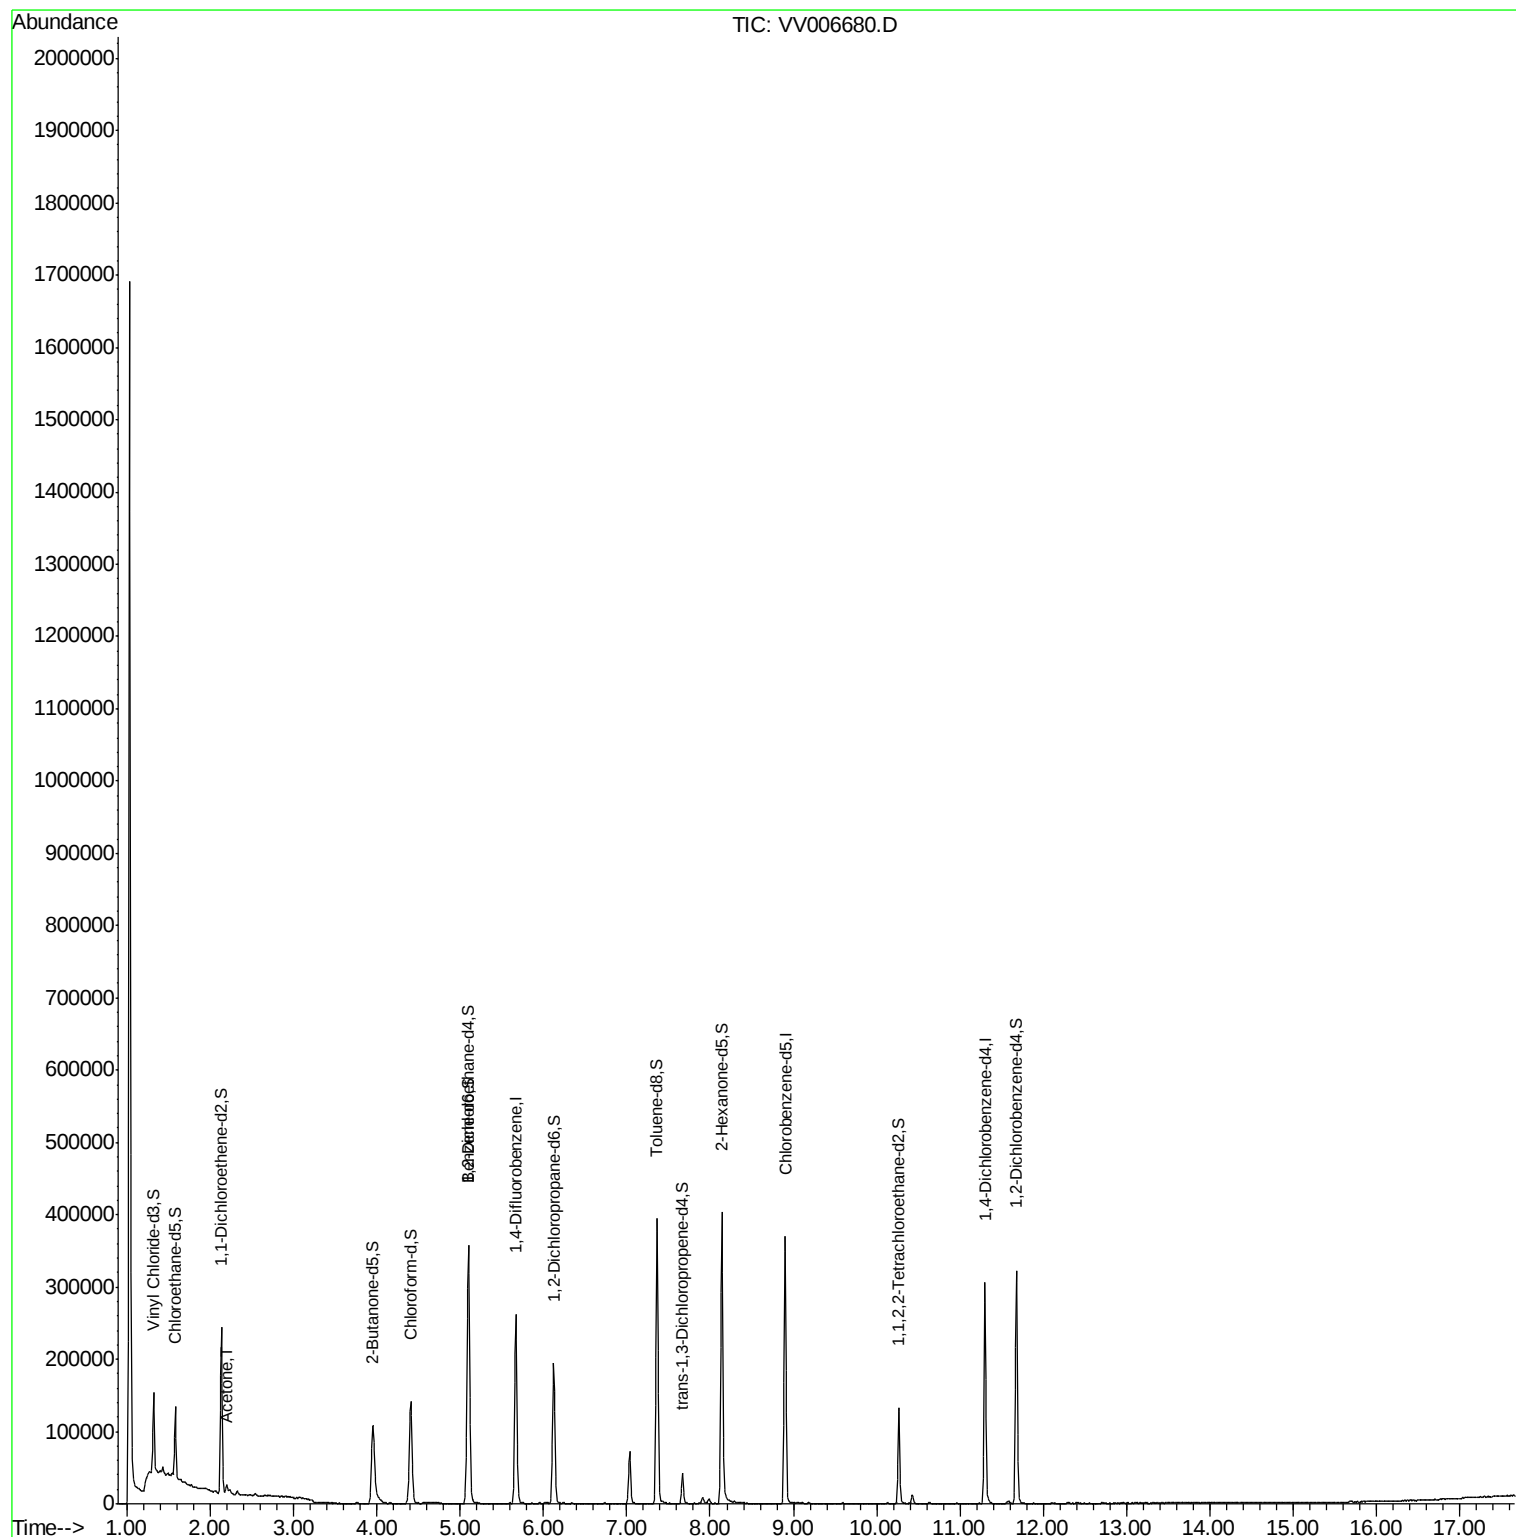

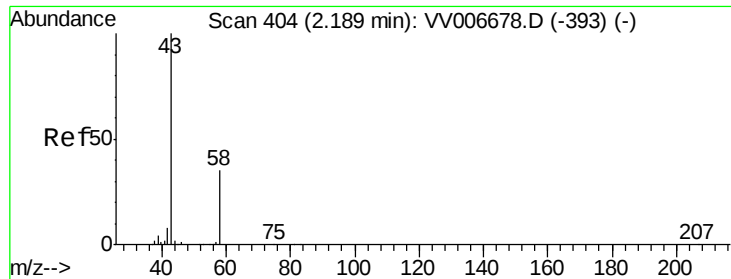

#13

Acetone

Concen: 3.55 ug/L

RT: 2.20 min Scan# 407

Delta R.T. 0.01 min

Lab File: VV006680.D

Acq: 21 Jul 2018 12:20

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Tot Ion: 43 Resp: 9463

Ion Ratio Lower Upper

43 100

58 35.5 0.0 72.8

