

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV072118\
 Data File : VV006681.D
 Acq On : 21 Jul 2018 12:47
 Operator : SY/MD
 Sample : J4078-07
 Misc : 25 mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB3

Quant Time: Jul 22 23:12:32 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jul 22 23:06:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	224456	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	205809	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	85193	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	84690	5.38	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.60%
7) Chloroethane-d5	1.58	69	65038	6.12	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	122.40%
11) 1,1-Dichloroethene-d2	2.13	63	121186	4.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.00%
20) 2-Butanone-d5	3.95	46	172259	50.35	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.70%
24) Chloroform-d	4.41	84	145549	5.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.80%
26) 1,2-Dichloroethane-d4	5.09	65	70058	5.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.00%
32) Benzene-d6	5.10	84	314033	5.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	112.40%
36) 1,2-Dichloropropane-d6	6.12	67	98028	5.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	113.00%
41) Toluene-d8	7.36	98	271462	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.40%
43) trans-1,3-Dichloropropene-	7.67	79	27173	4.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.40%
46) 2-Hexanone-d5	8.14	63	138722	47.31	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.62%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	63595	5.04	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	89223	5.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.40%


Target Compounds					Ovalue
13) Acetone	2.20	43	8319	3.17 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV072118\
Data File : VV006681.D
Acq On : 21 Jul 2018 12:47
Operator : SY/MD
Sample : J4078-07
Misc : 25 mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB3

Quant Time: Jul 22 23:12:32 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR071918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jul 22 23:06:02 2018
Response via : Initial Calibration

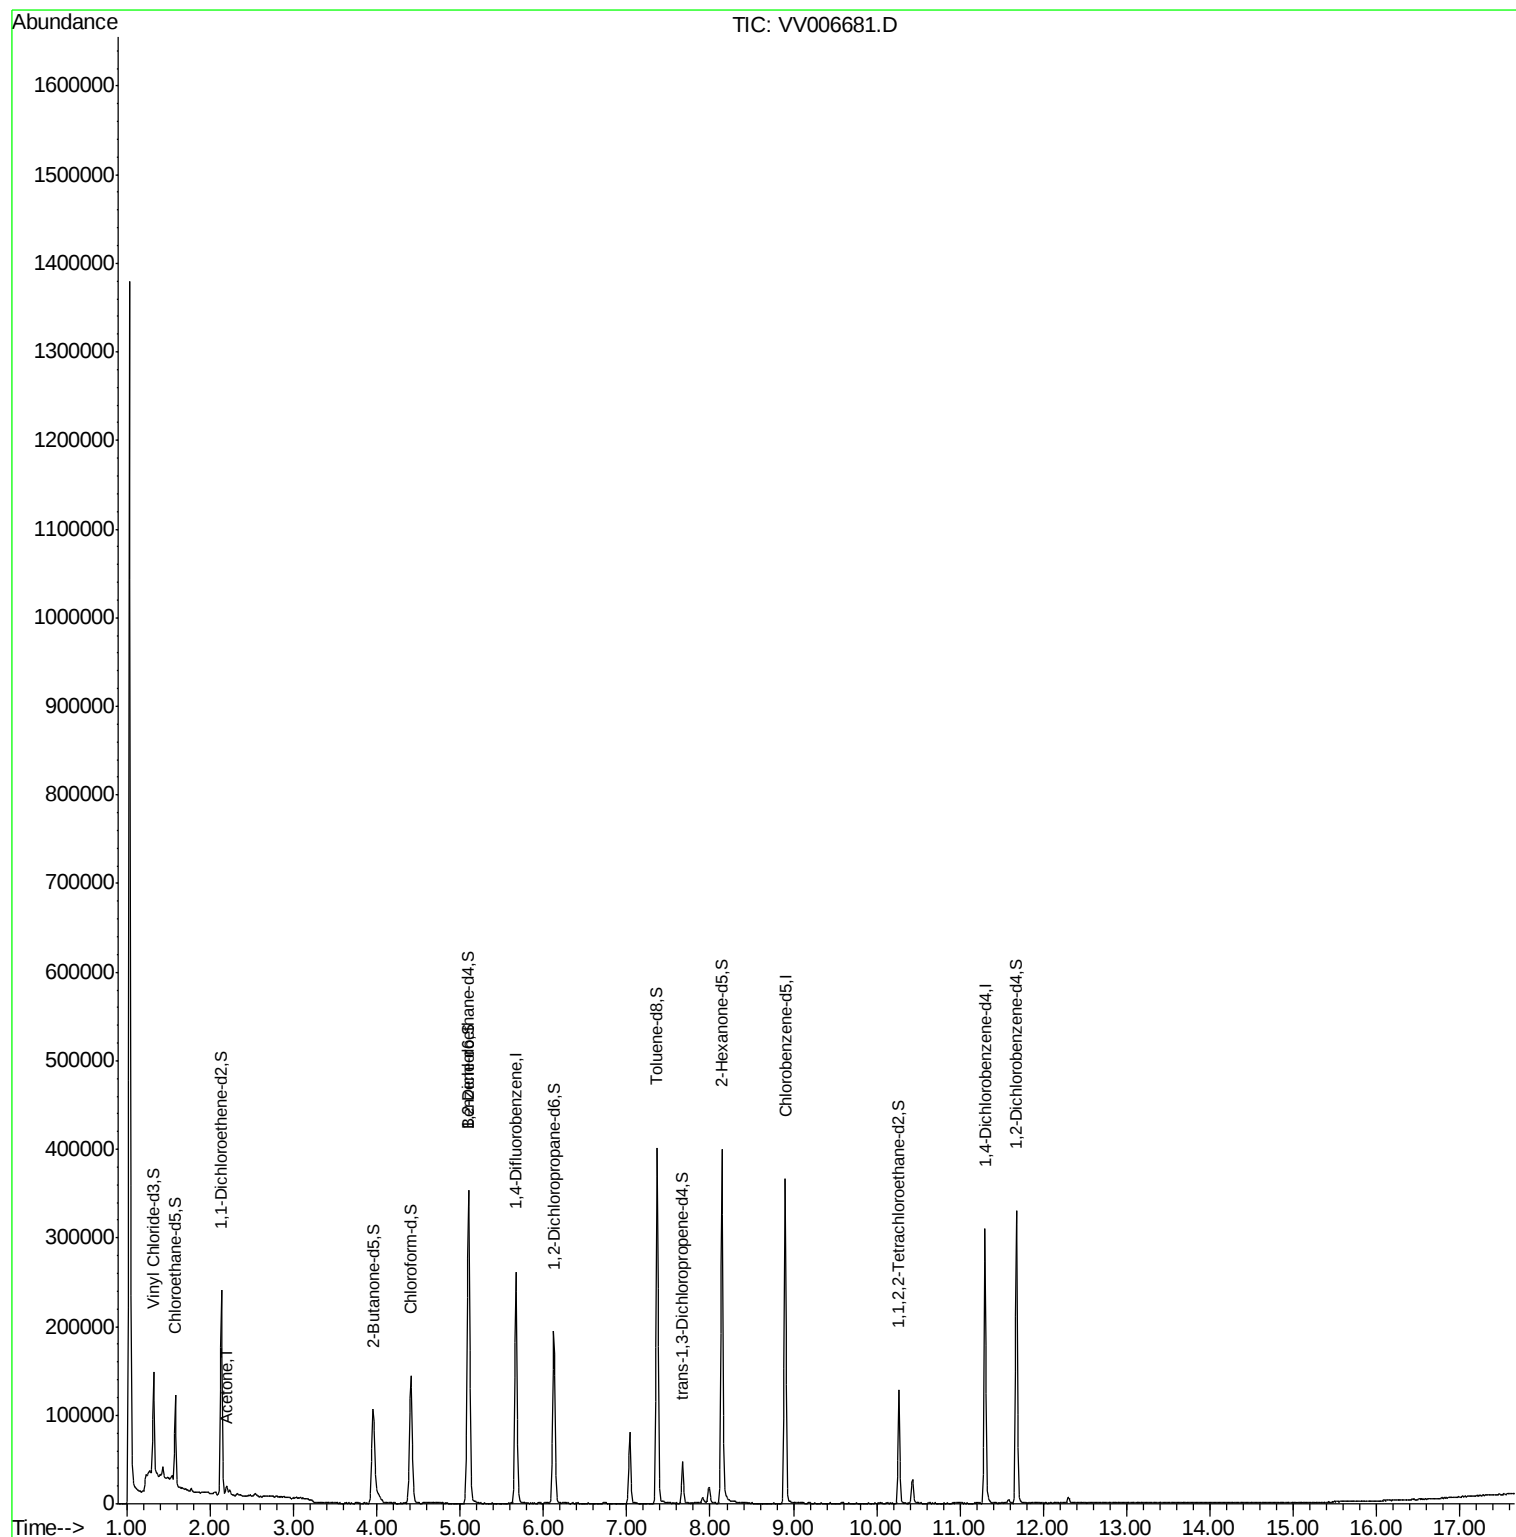

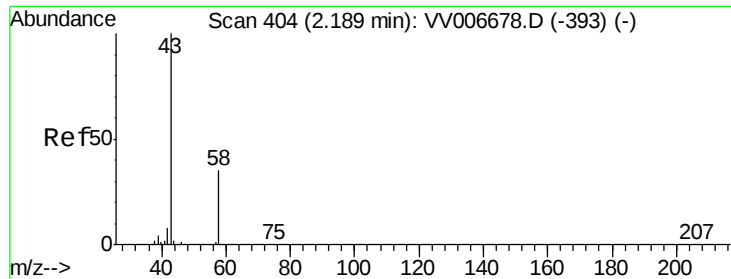

#13

Acetone

Concen: 3.17 ug/L

RT: 2.20 min Scan# 407

Delta R.T. 0.01 min

Lab File: VV006681.D

Acq: 21 Jul 2018 12:47

Instrument :
MSVOA_V
ClientSampleId :
C0AB3

Tot Ion: 43 Resp: 8319

Ion Ratio Lower Upper

43 100

58 35.2 0.0 72.8

